

HYCISUN[®]



Untersuchungshandschuhe Disposable Nitrile Exam Gloves



**EN
455**

**EN
374**

**EN
420**



Nitril / Puderfrei / Unsteril

Nitrile / Powder free / Non sterile

REF



SNVE10014



SNVE10015



SNVE10016



SNVE10017

HYCISIN® Untersuchungshandschuhe

Examination gloves
Powder free / Non sterile
Gants d'examen
Non poudrés / Non stérile
Guantes de examen
Sin polvo / No estériles
Onderzoekshandschoenen
Poedervrij / Niet steril

REF SNVE10015
BLAU / BLUE



Beachten Sie vor der Verwendung die Anweisungen und Vorichtsmaßnahmen auf der Verpackungsunterseite.
Consult the instructions and cautions on the bottom of the box before using.

OPEN HERE

Nitril
Pudertfrei / Unsteril
Medizin- & Schutzhandschuh

HYCISIN®
Untersuchungshandschuhe

Blau / Powder free / Unsteril
Medizin- & Schutzhandschuh

100 Stk.

Qualified acc. to
EN 374 & EN 455



CE

Beachten Sie vor der Verwendung die Anweisungen und Vorichtsmaßnahmen auf der Verpackungsunterseite.

EN EN
455 374

Medical Devices



6 322040 31713

Medical Devices

HYCISUN[®]

Untersuchungshandschuhe

Nitril / Puderfrei / Unsteril

Medizin- & Schutzhandschuh

100 Stk.



MD

AQL
1,0



EN EN
455 374

Beachten Sie vor der Verwendung die Anweisungen und
Vorsichtsmaßnahmen auf der Verpackungunterseite.

Medical Device



6 972940 817137

100 Stk.

Medizin- & Schutzhandschuh

Nitril / Puderfrei / Unsteril

Untersuchungshandschuhe

6 972940 817137



HYGISUN[®]

Untersuchungshandschuhe

Nitril / Puderfrei / Unsteril
Medizin- & Schutzhandschuh



Shandong INTCO Medical Products Co., Ltd.
www.intcomedical.com
Qiwang Road, Naoshan Industrial Park,
Qingzhou, Shandong, P.R. China



Lotus NL B.V.
Koningin Julianaplein 10, 1e Verd, 2595AA, The Hague, Netherlands.
peter@lotusnl.com

100 Stk.

M

Größe



Shandong INTCO Medical Products Co., Ltd.
www.intcomedical.com
Qiwang Road, Naoshan Industrial Park,
Qingzhou, Shandong, P.R. China



Lotus NL B.V.
Koningin Julianaplein 10, 1e Verd, 2595AA, The Hague, Netherlands.
peter@lotusnl.com

Importeur

Sunbeam International GmbH
Schumanstr. 12, 52146 Würselen,
Germany
Tel: 0049-2405-603980
Mail: info@sunbeam-international.de
www.hygisun.de

Größe

M

PPE Regulation (EU) / PSA-Verordnung (EU) 2016/425 (Cat. III): EN ISO 21420:2020
Product complies with Harmonized European Standards/ Produkt entspricht den harmonisierten europäischen Normen:
EN ISO 21420:2020, EN ISO 374-1:2016+A1:2018, EN ISO 374-5:2016, EN 16523-1:2015



KPI

| Code letter / Kennbuchstabe | Test chemical / Prüfchemikalie | EN ISO 374-1:2016 Permeation level / Leistungsstufen Permeation | EN ISO 374-4:2019 Mean degradation / Durchsichtliche Degradation |
|-----------------------------|--------------------------------------------|-----------------------------------------------------------------|------------------------------------------------------------------|
| K | Sodium hydroxide / Natriumhydroxid 40% | Level / Stufe 6 | -11.5% |
| P | Hydrogen peroxide / Wasserstoffperoxid 30% | Level / Stufe 2 | -9.5% |
| T | Formaldehyde / Formaldehyd 37% | Level / Stufe 3 | 7.4% |

Tested according to / Getestet gemäß EN 16523-1:2015

| Permeation level / Leistungsstufen Permeation EN ISO 374-1:2016+A1:2018 | 1 | 2 | 3 | 4 | 5 | 6 |
|----------------------------------------------------------------------------|-----|-----|-----|------|------|------|
| Minimum breakthrough time / Gemessene Durchbruchzeit (in min) | >10 | >30 | >60 | >120 | >240 | >480 |

Degradation levels indicate the change in puncture resistance of the gloves after exposure to the challenge chemical.
 Die Degradation gibt die Veränderung der Durchschlagsfestigkeit der Handschuhe nach ständigem Kontakt der Außenfläche mit der beanspruchenden Prüfchemikalie an.



Tested acc. to / Getestet gemäß
EN ISO 374-5:2016

CE 2777

Notified Body / Benannte Stelle:
SATRA Technology Europe Ltd.
 Bracetown Business Park, Clonee
 Dublin 15, Ireland
 (Notified Body 2777)

Declarations of conformity / further information are available at:
 Konformitätserklärung / weitere Informationen finden Sie unter:
www.hygisun.de/downloads

Die Degradation gibt die Veränderung der Durchschlagsfestigkeit der Handschuhe nach ständigem Kontakt der Außenfläche mit der beanspruchenden Prüfchemikalie an.
 EN ISO 374-1:2016+A1:2018
 EN ISO 374-5:2016

www.hygisun.de/downloads
 Konformitätserklärung / weitere Informationen finden Sie unter:
www.hygisun.de/downloads

HYCISUN[®]

Disposable Nitrile Exam Gloves

Nitrile / Powder free / Non sterile

Medical & Personal Protective

M
SIZE

LOT XXXXXX

2021-0X

202X-0X

S05X-0X

S054-0X

XXXXXXX

 **100 Pcs**

CE

CE

HYCISIN® Untersuchungshandschuhe

Examination gloves
Powder free / Non sterile
Gants d'examen
Non poudrés / Non stérile
Guantes de examen
Sin polvo / No esteriles
Onderzoekshandschoenen
Poedervrij / Niet steril

REF SNVE10015
BLAU / BLUE



Beachten Sie vor der Verwendung die Anweisungen und Vorichtsmaßnahmen auf der Verpackungsunterseite.
Consult the instructions and cautions on the bottom of the box before using.

Nitril
Pudertfrei / Unsteril
Medizin- & Schutzhandschuh

HYCISIN®
Untersuchungshandschuhe
Blau / Pudertfrei / Unsteril
Medizin- & Schutzhandschuh

100 Stk.



CE

Beachten Sie vor der Verwendung die Anweisungen und Vorichtsmaßnahmen auf der Verpackungsunterseite.

EN EN
455 374

Medical Device





HYGISUN®

Untersuchungshandschuhe

Nitril / Puderfrei / Unsteril
Medizin- & Schutzhandschuh



REF SNVE10015



EN 455

EN 374

AQL 1.5



BLAU

PPE Regulation (EU) / PSA-Verordnung (EU) 2016/425 (Cat. III): EN ISO 21420:2020
EN ISO 21420:2020, EN ISO 374-1:2016-A1:2019, EN ISO 374-5:2016, EN 16523-1:2015
 Product complies with Harmonised European Standard Product entspricht den harmonisierten europäischen Normen:

| Code user / Kontakttabelle | Test chemical / Pflanzensäfte | EN ISO 374-1:2016 Penetration level 1 | EN ISO 374-5:2016 Leakage | EN ISO 374-4:2016 Mean degradation Durchschnittliche Degradation |
|----------------------------------|-------------------------------------|------------------------------------------|------------------------------|------------------------------------------------------------------------|
| K | Sodium hypochlorite 40% | Level 1/ Stufe 6 | Level 1/ Stufe 6 | -11.5% |
| D | Hydrogen peroxide 6% | Level 1/ Stufe 2 | Level 1/ Stufe 2 | -9.0% |
| T | Formaldehyde 30% | Level 1/ Stufe 3 | Level 1/ Stufe 3 | 7.4% |

Tested according to: **General EN ISO EN 16523-2:2015**
EN ISO 214-1:2019-A1:2019
Minimum breakthrough time
Chemische Durchdringung (in min)

| | 1 | 2 | 3 | 4 | 5 | 6 |
|-----|-----|-----|------|------|------|---|
| >10 | +30 | +60 | +120 | +240 | +480 | |

Declaration levels indicate the change in puncture resistance of the gloves after exposure to the challenge chemical
 Die Degradation levels geben die Veränderung der Durchdringung der Handschuhe nach abgedehntem Kontakt der Außenseite mit der bestpraktischen Prüflösung an.

Tested acc. to / Getestet gemäß
EN ISO 374-5:2016



Notified Body / Benannte Stelle:
SATRA Technology Europe Ltd.
 Business Business Park, Clonsilla
 Dublin 15, Ireland
 (Notified Body 2777)

Declarations of conformity / further information are available at:
www.hygisun.de/downloads

CE 2777

Mass: 335mm X 260mm X 250mm
 Menge: 100 Packungen (100Stk./ Packung)



EAN (Box):



Lot# XXXXXX

2021-0X

202X-0X



Shandong NITCO Medical Products Co., Ltd.
www.nitco-med.com
 Diving Road, American Industrial Park,
 Qingdao, Shandong, P. R. China



Lotus NV B.V.
 Nieuwe Industrieweg 10, 1e. Vert. 2393AA The Hague, Netherlands
info@stapac.com



Sunbeam International GmbH
 Schürweg 12, 52246 Würselen, Germany
 Tel: +49 2402 993280
info@sunbeam-international.de
www.hygisun.de

EN ISO 21420:2020

| Code | Test | EN ISO 21420:2020 | EN ISO 21420:2020 | EN ISO 21420:2020 |
|------|-------------------------|-------------------|-------------------|-------------------|
| K | Sodium hypochlorite 40% | Level 1/ Stufe 6 | Level 1/ Stufe 6 | -11.5% |
| D | Hydrogen peroxide 6% | Level 1/ Stufe 2 | Level 1/ Stufe 2 | -9.0% |
| T | Formaldehyde 30% | Level 1/ Stufe 3 | Level 1/ Stufe 3 | 7.4% |

EN ISO 374-1:2016-A1:2019

| Code | Test | EN ISO 374-1:2016-A1:2019 | EN ISO 374-1:2016-A1:2019 | EN ISO 374-1:2016-A1:2019 |
|------|-------------------------|---------------------------|---------------------------|---------------------------|
| K | Sodium hypochlorite 40% | Level 1/ Stufe 6 | Level 1/ Stufe 6 | -11.5% |
| D | Hydrogen peroxide 6% | Level 1/ Stufe 2 | Level 1/ Stufe 2 | -9.0% |
| T | Formaldehyde 30% | Level 1/ Stufe 3 | Level 1/ Stufe 3 | 7.4% |

www.hygisun.de/downloads

www.hygisun.de
 info@stapac.com
 Tel: +49 2402 993280
 www.hygisun.de

202X-0X



Document Number : INTCO-CE-DC-NBR-001

Version: A/4

EU DECLARATION OF CONFORMITY

Manufacturer

Authorized Representative

Name: Shandong Intco Medical Products Co., Ltd.

Name: Lotus NL B.V.

Address: Qiwang Road, Naoshan Industrial Park, Qingzhou, Shandong, China

Address: Koningin Julianaplein 10, le Verd, 2595AA, The Hague, Netherlands

Declares that the MDR described hereafter

Product name and model:

Disposable Nitrile (NBR) Gloves

UMDNS code: 11882

Model: XS /S /M /L /XL/XXL

UDI-DI:

Meet the provisions of the Council Regulation EU 2017/745 and Annex I which apply to them.

The medical device has been assigned to Class I, based on rule 1 of Annex VIII Chapter III of the Regulation EU 2017/745 MDR. It bears the mark



This Declaration of conformity is valid for five years: 7 / May / 2020 to 6 / May / 2025. If there is a change in the declaration information, this declaration is invalid.

The above mentioned declaration of conformity is exclusively under the responsibility of

Company: Shandong Intco Medical Products Co., Ltd.

Address: Qiwang Road, Naoshan Industrial Park, Qingzhou, Shandong, China.

Shandong 2020-05-07

Place, date

Cui Zhongqiang Quality Manager

Legally binding signature, Function





Document Number : INTCO-CE-DC-NBR-001

Version: A/5

EU DECLARATION OF CONFORMITY

Manufacturer

Authorized Representative

Name: Shandong Intco Medical Products Co., Ltd.
Address: Qiwang Road NO.9888, Naoshan Industrial Park, Qingzhou, Shandong, China

Name: Lotus NL B.V.
Address: Koningin Julianaplein 10, 1e Verd, 2595AA, The Hague, Netherlands

Declares that the MDR described hereafter

Product name and model:

Disposable Nitrile Exam Gloves

EMDN code: T01020204

Model: XS /S /M /L /XL/XXL

Product Code: NGV/B/H/PEM 10013-10018, NGV/B/H/PEM 10023-10028, NGV/B/H/PEM 10033-10038, NGV/B/H/PEM 10043-10048, NGV/B/H/PEM 10053-10058.

Basic UDI-DI: 697024575Nitrile7G

SRN: CN-MF-000002100

This Declaration of Conformity is issued under the sole responsibility of the manufacturer:
Shandong Intco Medical Products Co., Ltd.

Conformity Assessment Route: Annex II and Annex III according to EU 2017/745.

Applicable Standard:

EN ISO 13485:2016; EN 14971:2019; EN 1041:2008; EN 15223-1:2016;

EN 455-1:2020; EN 455-2:2015; EN 455-3:2015; EN 455-4:2009;

ISO 10993-1:2018; ISO 10993-10:2010. ISO 10993-11:2017.

Meet the provisions of the Council Regulation EU 2017/745 and Annex I which apply to them,

The medical device has been assigned to Class I, based on rule 1 & rule 5 of Annex VIII

Chapter III of the Regulation EU 2017/745 MDR. It bears the mark



We agree to develop, implement and maintain a documented post-production monitoring process.

Shandong 2021-04-12

Place, date

Rick Cheng

Rick Cheng Quality Manager

Legally binding signature, Function



CERTIFICATE OF REGISTRATION

This is to certify that the management system of:

Shandong Intco Medical Products Co., Ltd.

Main Site: Qiwang Road No.9888, Naoshan Industrial Park, Qingzhou
City, Shandong Province, 262500, P. R. China

has been registered by Intertek as conforming to the requirements of:

ISO 13485:2016

The management system is applicable to:

Manufacture of non-sterile NBR (Nitrile Butadiene Rubber) and PVC (Poly
Vinyl Chloride) medical examination gloves.

Certificate Number:

0086238-01

Initial Certification Date:

28 April 2014

Date of Certification Decision:

9 January 2021

Issuing Date:

9 January 2021

Valid Until:

31 December 2021



Intertek



A handwritten signature in black ink, appearing to read "Calin Moldovean".

Calin Moldovean

President, Business Assurance

Intertek Testing Services NA Ltd.,
1829, 32nd avenue, Lachine, QC, H8T 3J1,
Canada



CERTIFICATE OF REGISTRATION

This is to certify that the management system of:

Shandong Intco Medical Products Co., Ltd

No.9888, Qiwang Road, Naoshan Industrial Park, Qingzhou City, Shandong
Province, P. R. China

has been registered by Intertek as conforming to the requirements of:

ISO 9001:2015

The management system is applicable to:

Manufacturing of disposable non sterile NBR (Nitrile Butadiene Rubber) and
PVC (Poly Vinyl Chloride) gloves and disposable face masks (Non-medical)

*(Organization was certified by another Certification Body before
2019/01/03)*

Unified Social Credit Identifier:

91370781561439654L

Certificate Number:

111812005

Initial Certification Date:

27 January 2013

Date of Certification Decision:

23 December 2020

Certified by Intertek since:

03 January 2019

Issuing Date:

23 December 2020

Valid Until:

27 January 2022



Intertek

014

Calin Moldovean

President, Business Assurance

Intertek Certification Limited, 10A Victory
Park, Victory Road, Derby DE24 8ZF, United
Kingdom

Intertek Certification Limited is a
UKAS accredited body under
schedule of accreditation no. 014.





Issued to:

Shandong Intco Medical Products Co Ltd
Qiwang Road, Naoshan Industrial Park
Qingzhou
Shandong
262506
China

Notified Body: 2777

SATRA customer number: P1720

EU Type-Examination Certificate

Certificate number: 2777/17447-02/E00-00

This EU Type-Examination Certificate covers the following product group(s) supported by testing to the relevant standards/technical specifications and examination of the technical file documentation:

Following the EU Type-Examination this product group has been shown to satisfy the applicable essential health and safety requirements of Annex II of the PPE Regulation (EU) 2016/425 as a Category III product.

Product reference:

Description:

| | | |
|-----------------|----------------------------------------------------------|-----------------------|
| NGV/B/H/P/XE100 | Disposable Nitrile Gloves/ SYNGUARD® Nitrile Exam Gloves | |
| NGV/B/H/P/XE200 | Blue | Black |
| SNV/B/H/PE100 | NGV/B/H/P/XE100 13-18 | NGV/B/H/P/XE100 43-48 |
| SNV/B/H/PE200 | NGV/B/H/P/XE200 13-18 | NGV/B/H/P/XE200 43-48 |
| | SNV/B/H/PE100 13-18 | SNV/B/H/PE100 43-48 |
| | SNV/B/H/PE200 13-18 | SNV/B/H/PE200 43-48 |
| | White | Violet |
| | NGV/B/H/P/XE100 23-28 | NGV/B/H/P/XE100 33-38 |
| | NGV/B/H/P/XE200 23-28 | NGV/B/H/P/XE200 33-38 |
| | SNV/B/H/PE100 23-28 | SNV/B/H/PE100 33-38 |
| | SNV/B/H/PE200 23-28 | SNV/B/H/PE200 33-38 |

Sizes:

6-11(XS-XXL)

Classification:

EN ISO 374-1:2016+A1:2018/Type B

Level

EN ISO 374-4:2019

Degradation %

(K) Sodium hydroxide 40%
(P) Hydrogen peroxide 30%
(T) Formaldehyde 37%

6
2
3

-11.5
-9.5
7.4

EN ISO 374-5:2016

Protection against Bacterial and Fungi
Protection against Viruses

Level

Pass
Pass

Standards/Technical specifications applied:

EN ISO 21420:2020; EN ISO 374-1:2016+A1:2018; EN ISO 374-5:2016

Technical reports/Approval documents:

SATRA: CHT0291374/1944, CHM0291937/1946/JH, CHT0301241/2033

SGS: CH:TX:9420026599-1, CH:TX:9420026316-1, CH:TX:9420020333, CH:TX:9420029243

CTC: S200908976_2

TUV: 721655656

Date first issued: 15/07/2021

Date of issue: 20/07/2021

Expiry date: 15/07/2026

Signed on behalf of SATRA:

Geoff Graham

TERMS AND CONDITIONS

The following conditions apply in addition to SATRA's standard terms and conditions of business and those given in the current certification agreement. This certificate has been issued in accordance with Annex V (Module B) of the applicable legislation (see note 11).

Please note:

1. Where the product is classified as category III then CE or UKCA Marking of production is reliant on current compliance with module C2 or Module D of the applicable legislation (See note 11). (Except that specifically produced to fit an individual user).
2. Full details of the scope of the certification and product(s) certified are contained within the manufacturer's technical documentation.
3. Where a translation of this certificate exists, the English language version shall be considered as the authoritative text.
4. Certification is limited to production undertaken at the sites listed in the manufacturer's technical documentation.
5. Ongoing manufactured product shall be consistent with the product(s) certified and listed on this certificate and an EU declaration of product conformity shall be made available in accordance with the applicable legislation (See note 11)
6. The Manufacturer shall inform SATRA of any changes to the certified product or technical documentation.
7. Where results obtained during type testing are within the budget of uncertainty when compared to the pass requirement, classification or performance level, then it is the responsibility of the manufacturer to ensure that the factory production control and manufacturing tolerances are such that the product placed on the market meets with the stated requirements, classifications or performance levels.
8. This certificate shall be kept together with the relevant technical documentation in a safe place by the client named on this certificate. Production of this certificate and other documentation may be required by a representative of the EC member state, or UK government.
9. This certificate relates only to the condition of the testable items at the time of the certification procedure and is subject to the expiry date shown.
10. SATRA reserves the right to withdraw this certificate if it is found that a condition of manufacture, design, materials or packaging have been changed and therefore no longer comply with the requirements of the applicable legislation (See note 11).
11. These terms and conditions shall apply to the requirements set out in Regulation (EU) 2016/425 of the European Parliament and of the council of 9th March 2016 on personal protective equipment or to UK legislation relating to UKCA Marking as defined within the issued certificate.

Test Report No. 7191205302-EEC19-WBH
dated 01 Mar 2019



PSB Singapore

**Add value.
Inspire trust.**

Note: This report is issued subject to the Testing and Certification Regulations of the TÜV SÜD Group and the General Terms and Conditions of Business of TÜV SÜD PSB Pte Ltd. In addition, this report is governed by the terms set out within this report.

SUBJECT:

Testing of Disposable Nitrile Glove submitted by
Shandong Intco Medical Products Co., Ltd. on 18 Feb 2019.

TESTED FOR:

Shandong Intco Medical Products Co., Ltd
No. 9888 Qiwang Road
Naoshan Industry Park, Qingzhou, Shandong, China

TEST DATE:

25 Feb 2019

DESCRIPTION OF SAMPLES:

| S/N | Product Description | Colour | Lot No. | Size | Sample received (pieces) | Manufacturer |
|-----|--------------------------|--------|---------|------|--------------------------|------------------------------------------|
| 1 | Disposable Nitrile Glove | Blue | / | M | 217 | Shandong Intco Medical Products Co., Ltd |

Lot size as specified by client: 35,001 to 150,000 pieces

METHOD OF TEST:

EN 455-1:2000 Medical gloves for single use
Part 1: Requirements and testing for freedom from holes



Laboratory:
TÜV SÜD PSB Pte. Ltd.
No.1 Science Park Drive
Singapore 118221

Phone : +65-6885 1333
Fax : +65-6776 8670
E-mail: enquiries@tuv-sud-psb.sg
www.tuv-sud-psb.sg
Co. Reg : 199002667R

Regional Head Office:
TÜV SÜD Asia Pacific Pte. Ltd.
1 Science Park Drive, #02-01
Singapore 118221
TUV®

Test Report No. 7191205302-EEC19-WBH
dated 01 Mar 2019



PSB Singapore

RESULTS:


Sample: Disposable Nitrile Glove, Size M

Table: Results for EN 455-1:2000

| Clause | Tests | Requirements | No. of non-compliers allowed (pieces) | Number tested (pieces) | Actual no. of non-compliers found (pieces) | Inferred results |
|--------|--------------------|----------------|---------------------------------------|------------------------|--------------------------------------------|------------------|
| 4 5 | Freedom from holes | Shall not leak | 7 | 200 | 0 | Passed |

REMARKS:

1. The manufacturing lot no. was not provided by the client.



Yeo Poh Kwang
Higher Associate Engineer



Wong Bee Hui
Product Manager
Medical Health Services (NAM)

APPENDIX:



Photo : Disposable Nitrile Glove, Size M

Please note that this Report is issued under the following terms :

1. This report applies to the sample of the specific product/equipment given at the time of its testing/calibration. The results are not used to indicate or imply that they are applicable to other similar items. In addition, such results must not be used to indicate or imply that TÜV SÜD PSB approves, recommends or endorses the manufacturer, supplier or user of such product/equipment, or that TÜV SÜD PSB in any way "guarantees" the later performance of the product/equipment. Unless otherwise stated in this report, no tests were conducted to determine long term effects of using the specific product/equipment.
2. The sample/s mentioned in this report is/are submitted/supplied/manufactured by the Client. TÜV SÜD PSB therefore assumes no responsibility for the accuracy of information on the brand name, model number, origin of manufacture, consignment or any information supplied.
3. Nothing in this report shall be interpreted to mean that TÜV SÜD PSB has verified or ascertained any endorsement or marks from any other testing authority or bodies that may be found on that sample.
4. This report shall not be reproduced wholly or in parts and no reference shall be made by the Client to TÜV SÜD PSB or to the report or results furnished by TÜV SÜD PSB in any advertisements or sales promotion.
5. Unless otherwise stated, the tests were carried out in TÜV SÜD PSB Pte Ltd, No.1 Science Park Drive Singapore 118221.

July 2011



Test Report No. 7191255592-EEC21-WBH
dated 31 Mar 2021



PSB Singapore

**Add value.
Inspire trust.**

Note: This report is issued subject to the Testing and Certification Regulations of the TÜV SÜD Group and the General Terms and Conditions of Business of TÜV SÜD PSB Pte Ltd. In addition, this report is governed by the terms set out within this report.

SUBJECT:

Testing of Examination Gloves submitted by
Shandong Intco Medical Products Co., Ltd. on 10 Mar 2021

TESTED FOR:

Shandong Intco Medical Products Co., Ltd.
No. 9888 Qiwang Road,
Naoshan Industry Park,
Qingzhou, Shandong,
China

TEST DATE:

12 Mar 2021 to 31 Mar 2021

DESCRIPTION OF SAMPLES:

| S/N | Product Description | Brand/ Model | Colour | Lot No. | Size | Sample received (pieces) | Manufacturer |
|-----|---------------------------------------|--------------|--------|---------|------|--------------------------|-------------------------------------------|
| 1 | Disposable Nitrile Examination Gloves | Nil | Blue | Nil | S | 15 | Shandong Intco Medical Products Co., Ltd. |
| 2 | | | | Nil | M | 32 | |
| 3 | | | | Nil | L | 15 | |
| 4 | | | | Nil | XL | 15 | |

METHOD OF TEST:

EN 455-2:2015 Medical gloves for single use
Part 2: Requirements and testing for physical properties
-Clause 4 Dimensions
-Clause 5 Strength



Laboratory:
TÜV SÜD PSB Pte. Ltd.
15 International Business Park
TÜV SÜD @ IBP
Singapore 609937

Phone : +65-6778 7777
E-mail: info.sg@tuvsud.com
<https://www.tuvsud.com/sg>
Co. Reg : 199002667R

Regional Head Office:
TÜV SÜD Asia Pacific Pte. Ltd.
15 International Business Park
TÜV SÜD @ IBP
Singapore 609937
TUV®

Test Report No. 7191255592-EEC21-WBH
dated 31 Mar 2021



PSB Singapore

RESULTS:


Sample: Disposable Nitrile Examination Gloves

Table: Results for EN 455-2:2015 Clauses 4-5

| Clause | Tests | Size | Requirements (Median) | Number tested (pieces) | Results (Median) | Inferred results |
|--------|------------------------------------------------------------------|------|------------------------------------------|------------------------|------------------|------------------|
| 4 | Dimensions a) Length (mm) | S | ≥ 240 | 13 | 248 | Passed |
| | | M | | 13 | 243 | Passed |
| | | L | | 13 | 248 | Passed |
| | | XL | | 13 | 250 | Passed |
| | b) Width (mm) | S | 80 ± 10 | 13 | 83 | Passed |
| | | M | 95 ± 10 | 13 | 98 | Passed |
| | | L | 110 ± 10 | 13 | 105 | Passed |
| | | XL | ≥ 110 | 13 | 110 | Passed |
| 5 | a) Force at break (N) | M | For nitrile examination gloves: ≥ 6.0 | 13 | 6.5 | Passed |
| | b) Force at break after challenge testing (N) 7 days at (70±2)°C | M | For nitrile examination gloves: ≥ 6.0 | 13 | 6.3 | Passed |

REMARKS:

- Brand/ Model and Lot No. were not provided by client.



Yeo Poh Kwang
Associate Engineer



Wong Bee Hui
Product Manager
Medical Health Services (NAM)

APPENDIX:

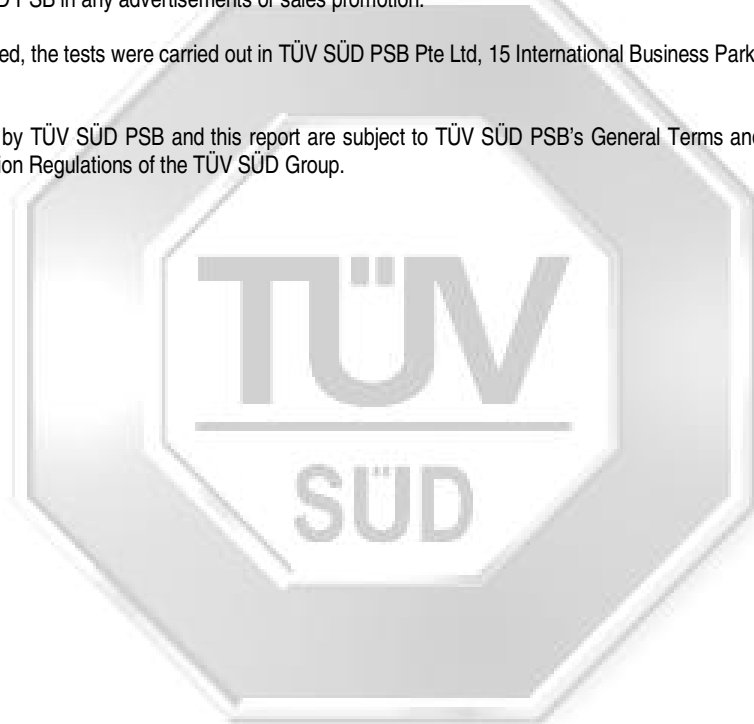


Photo: Disposable Nitrile Examination Gloves

Please note that this Report is issued under the following terms :

1. This report applies to the sample of the specific product/equipment given at the time of its testing/calibration. The results are not used to indicate or imply that they are applicable to other similar items. In addition, such results must not be used to indicate or imply that TÜV SÜD PSB approves, recommends or endorses the manufacturer, supplier or user of such product/equipment, or that TÜV SÜD PSB in any way "guarantees" the later performance of the product/equipment. Unless otherwise stated in this report, no tests were conducted to determine long term effects of using the specific product/equipment.
2. The sample/s mentioned in this report is/are submitted/supplied/manufactured by the Client. TÜV SÜD PSB therefore assumes no responsibility for the accuracy of information on the brand name, model number, origin of manufacture, consignment or any information supplied.
3. Nothing in this report shall be interpreted to mean that TÜV SÜD PSB has verified or ascertained any endorsement or marks from any other testing authority or bodies that may be found on that sample.
4. This report shall not be reproduced wholly or in parts and no reference shall be made by the Client to TÜV SÜD PSB or to the report or results furnished by TÜV SÜD PSB in any advertisements or sales promotion.
5. Unless otherwise stated, the tests were carried out in TÜV SÜD PSB Pte Ltd, 15 International Business Park TÜV SÜD @ IBP Singapore 609937.
6. The tests carried out by TÜV SÜD PSB and this report are subject to TÜV SÜD PSB's General Terms and Conditions of Business and the Testing and Certification Regulations of the TÜV SÜD Group.

Effective 26 January 2021



Test Report No. 7191256089-EEC21-WBH
dated 31 Mar 2021



PSB Singapore

**Add value.
Inspire trust.**

Note: This report is issued subject to the Testing and Certification Regulations of the TÜV SÜD Group and the General Terms and Conditions of Business of TÜV SÜD PSB Pte Ltd. In addition, this report is governed by the terms set out within this report.

SUBJECT:

Testing of Examination Gloves submitted by
Shandong Intco Medical Products Co., Ltd. on 15 Mar 2021

TESTED FOR:

Shandong Intco Medical Products Co., Ltd.
No. 9888 Qiwang Road,
Naoshan Industry Park,
Qingzhou, Shandong,
China

TEST DATE:

17 Mar 2021 to 31 Mar 2021

DESCRIPTION OF SAMPLES:

| S/N | Product Description | Brand/ Model | Colour | Lot No. | Size | Sample received (pieces) | Manufacturer |
|-----|---------------------------------------|--------------|--------|---------|------|--------------------------|-------------------------------------------|
| 1 | Disposable Nitrile Examination Gloves | Nil | Blue | Nil | S | 34 | Shandong Intco Medical Products Co., Ltd. |
| 2 | | | | Nil | L | 35 | |
| 3 | | | | Nil | XL | 34 | |

METHOD OF TEST:

EN 455-2:2015 Medical gloves for single use
Part 2: Requirements and testing for physical properties
-Clause 4 Dimensions
-Clause 5 Strength



Laboratory:
TÜV SÜD PSB Pte. Ltd.
15 International Business Park
TÜV SÜD @ IBP
Singapore 609937

Phone : +65-6778 7777
E-mail: info.sg@tuvsud.com
<https://www.tuvsud.com/sg>
Co. Reg : 199002667R

Regional Head Office:
TÜV SÜD Asia Pacific Pte. Ltd.
15 International Business Park
TÜV SÜD @ IBP
Singapore 609937
TUV®

Test Report No. 7191256089-EEC21-WBH
dated 31 Mar 2021



PSB Singapore

RESULTS:


Sample: Disposable Nitrile Examination Gloves

Table: Results for EN 455-2:2015 Clauses 4-5

| Clause | Tests | Size | Requirements (Median) | Number tested (pieces) | Results (Median) | Inferred results |
|--------|------------------------------------------------------------------|------|---------------------------------------|------------------------|------------------|------------------|
| 4 | Dimensions a) Length (mm) | S | ≥ 240 | 13 | 248 | Passed |
| | | L | | 13 | 252 | Passed |
| | | XL | | 13 | 246 | Passed |
| | b) Width (mm) | S | 80 ± 10 | 13 | 84 | Passed |
| | | L | 110 ± 10 | 13 | 104 | Passed |
| | | XL | ≥ 110 | 13 | 115 | Passed |
| 5 | Strength a) Force at break (N) | S | For nitrile examination gloves: ≥ 6.0 | 13 | 6.1 | Passed |
| | | L | | 13 | 6.4 | Passed |
| | | XL | | 13 | 6.3 | Passed |
| | b) Force at break after challenge testing (N) 7 days at (70±2)°C | S | For nitrile examination gloves: ≥ 6.0 | 13 | 7.0 | Passed |
| | | L | | 13 | 6.9 | Passed |
| | | XL | | 13 | 6.6 | Passed |

REMARKS:

- Brand/ Model and Lot No. were not provided by client.



Yeo Poh Kwang
Associate Engineer



Wong Bee Hui
Product Manager
Medical Health Services (NAM)

APPENDIX:

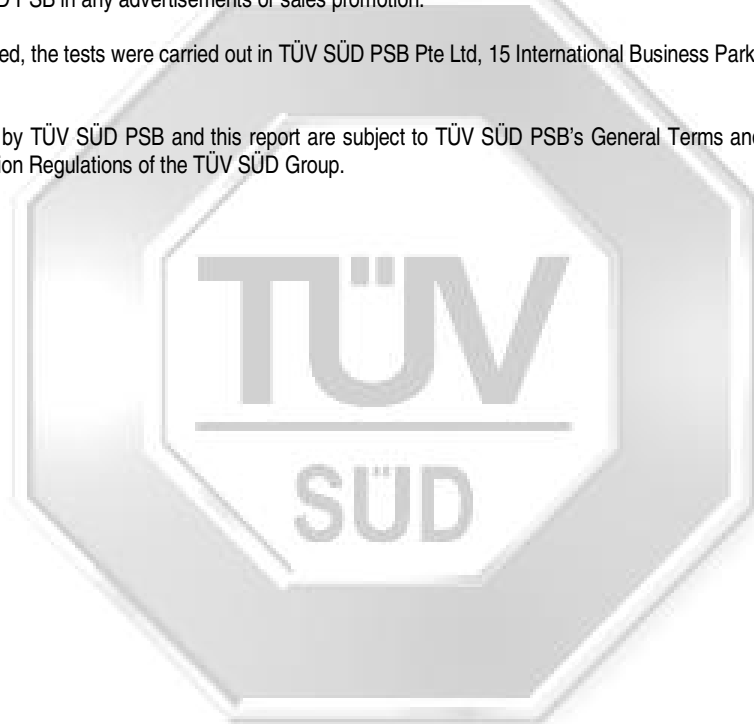


Photo: Disposable Nitrile Examination Gloves

Please note that this Report is issued under the following terms :

1. This report applies to the sample of the specific product/equipment given at the time of its testing/calibration. The results are not used to indicate or imply that they are applicable to other similar items. In addition, such results must not be used to indicate or imply that TÜV SÜD PSB approves, recommends or endorses the manufacturer, supplier or user of such product/equipment, or that TÜV SÜD PSB in any way "guarantees" the later performance of the product/equipment. Unless otherwise stated in this report, no tests were conducted to determine long term effects of using the specific product/equipment.
2. The sample/s mentioned in this report is/are submitted/supplied/manufactured by the Client. TÜV SÜD PSB therefore assumes no responsibility for the accuracy of information on the brand name, model number, origin of manufacture, consignment or any information supplied.
3. Nothing in this report shall be interpreted to mean that TÜV SÜD PSB has verified or ascertained any endorsement or marks from any other testing authority or bodies that may be found on that sample.
4. This report shall not be reproduced wholly or in parts and no reference shall be made by the Client to TÜV SÜD PSB or to the report or results furnished by TÜV SÜD PSB in any advertisements or sales promotion.
5. Unless otherwise stated, the tests were carried out in TÜV SÜD PSB Pte Ltd, 15 International Business Park TÜV SÜD @ IBP Singapore 609937.
6. The tests carried out by TÜV SÜD PSB and this report are subject to TÜV SÜD PSB's General Terms and Conditions of Business and the Testing and Certification Regulations of the TÜV SÜD Group.

Effective 26 January 2021





Material and Engineering Laboratory-Kaohsiung

Test Report



Report No. : KV-18-11251
Page No. : 1 OF 2
Date of Report : Dec. 25, 2018

Shandong Intco Medical Products Co., Ltd.

No.9888, Qiwang Road, Naoshan Industry Park, Qingzhou, Shandong, China

| | |
|---------------------------------------|---------------------------------------------------------------------------------------------------------------------------|
| <u>Product Name</u> | Disposable Nitrile Glove (QDHL1811025521OT) |
| <u>Date of Sample Received</u> | Dec. 10, 2018 |
| <u>Date of Testing</u> | Dec. 10, 2018~Dec. 25, 2018 |
| <u>Remark</u> | The information mentioned in the above section is provided by Client(Exclude Date of Sample Received and Date of Testing) |

=====
The laboratory tests according to the test requests and samples provided by client, and the results are as follows:


Test Request : Aqueous Extractable Protein

Test Method : Refer to BS EN 455-3:2015 Medical gloves for single use —
Part 3 : Requirements and testing for biological evaluation

Test Result : Please see attached pages

----- 1 -----

The required specification(s) offered in this test report is/are for reference only.
The conformity judgment is at the Applicant's final verdict.


Signed for and on behalf of
SGS Taiwan Ltd.

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested.

Test Report



Report No. : KV-18-11251

Page No. : 2 OF 2

Date of Report : Dec. 25, 2018

Test Equipment :

| Name | Brand | Model |
|------------------------------|----------|---------|
| UV-VISIBLE Spectrophotometer | SHIMADZU | UV-1700 |

Lab. Environmental Conditions:

Ambient Temperature : (25 ± 2) °C

Relative humidity : (50 ± 10) %


Test Result :

| INSPECTION ITEM | TEST RESULT |
|-----------------------------------|-------------|
| Aqueous Extractable Protein (ppm) | n.d. |

Note: 1. n.d. = not detected.

2. MDL (METHOD DETECTION LIMIT):0.2ppm.

Sample Photo :

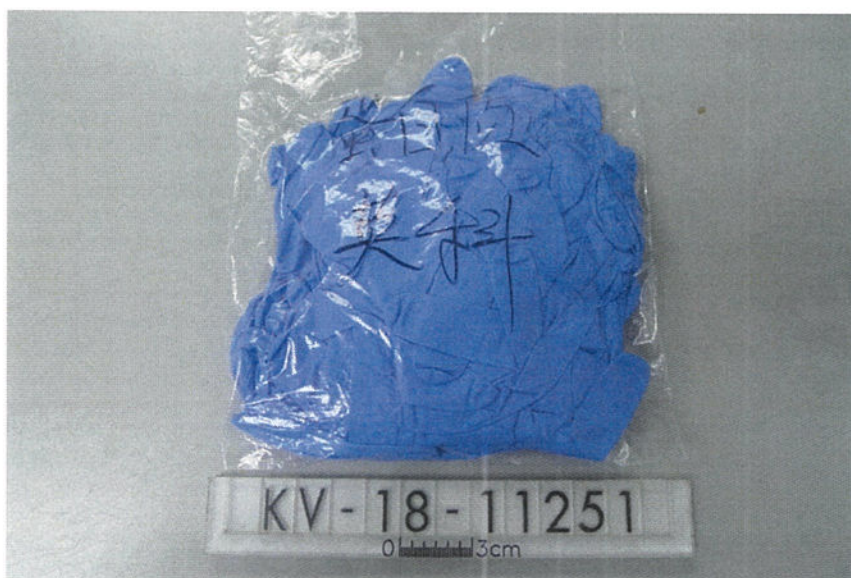

----- oOo -----

The required specification(s) offered in this test report is/are for reference only.
The conformity judgment is at the Applicant's final verdict.

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested.

SGS



中国认可
国际互认
检测
TESTING
CNAS L0604

scan to see the report



QDHL2103500009MD

Test Report

Report No.: QDHL2103500009MD

Sample Description: DISPOSABLE NITRILE EXAM GLOVES

Applicant: SHANDONG INTCO MEDICAL
PRODUCTS CO., LTD

Test Type: SUBMITTED BY CLIENT

SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.

Page 1 of 6

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.



QD 7442591

SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.

SGS Center, No.143, Zhuzhou Road, Laoshan District, Qingdao, Shandong, China 266101

t (86-532) 68999888

www.sgsgroup.com.cn

sgs.china@sgs.com

Member of the SGS Group (SGS SA)

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755)85071443, or email: CN.Doccheck@sgs.com

Report No.: QDHL2103500009MD

Test Report

| | | | | |
|--------------------|-----------------------------------------------------|-------------------------------------------------------------------|------------------------------------------|--------------|
| Sample information | Sample Description | DISPOSABLE NITRILE EXAM GLOVES | Color | NOT PROVIDED |
| | Received sample quantity/ Tested sample quantity | 10PCS/ 5PCS | Type/ Specifications | S |
| | Lot No. | NOT PROVIDED | Lot Quantity | NOT PROVIDED |
| | Manufacture Date | NOT PROVIDED | Expiration Date | NOT PROVIDED |
| | Material/Appearance | NOT PROVIDED | Storage Condition | NOT PROVIDED |
| | Manufacturer | NOT PROVIDED | | |
| | Others | NOT PROVIDED | | |
| | Client information | Applicant | SHANDONG INTCO MEDICAL PRODUCTS CO., LTD | |
| Applicant address | | NO.9888,QIWANG ROAD,NAOSHAN INDUSTRY PARK,QINGZHOU,SHANDONG,CHINA | | |

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755)83071443, or email: CN.Doccheck@sgs.com

SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.
Page 2 of 6

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of a Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.



Report No.: QDHL2103500009MD

| | | | | |
|------------------|----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------|------------------|----------------------------|
| Test information | Sample Receiving Date | MAR.01,2021 | Test Period Date | MAR.01,2021 TO MAR.05,2021 |
| | Sample No. | QDHL2103500009MD | Test environment | Meet requirement |
| | Test items | Removable surface powder | | |
| | Testing Accordance | EN 455-3:2015 Medical Gloves for Single Use-Part 3: Requirements and Testing for Biological Evaluation clause 4.4 | | |
| Test conclusion | This report only provides the test results and individual judgment, conclusion please see follow pages. Issue date: MAR.05,2021 | | | |
| Remark | / | | | |

Approver: *Joske Bao* Auditor: *Jenice Bao* Compiler: *William Diao*
 Date: 2021.03.05 Date: 2021.03.05 Date: 2021.03.05

SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.
Page 3 of 6


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

QD 7442593



Report No.: QDHL2103500009MD

Sample Photo

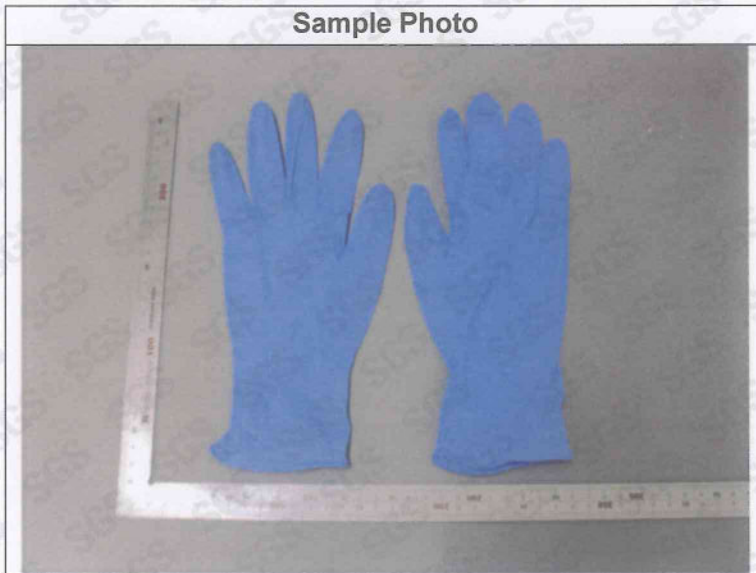

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755)83071443, or email: CN.Doccheck@sgs.com

SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.
Page 4 of 6

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.



QD 7442594

Report No.: QDHL2103500009MD

Test Results

| Test Items | Unit | Test Method | Requirement | Test Result | Assessment |
|--------------------------|------|----------------------------------------------------|-------------|-------------|------------|
| Removable surface powder | mg | EN 455-3: 2015 Clause 5.2 EN ISO 21171: 2006 | ≤2 | 0.22 | Pass |

Remarks:

1. Finish of gloves: Powdered-free gloves (As per client's requirement).
2. The declaration of conformity is only based on the actual value of laboratory activity, measurement uncertainty of the results not take into account.

End of Report

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755)83071443, or email: CN.Doc@sgs.com

SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.
Page 5 of 6

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.



SGS



中国认可
国际互认
检测
TESTING
CNAS L0604

Statement

1. The report is considered invalidated in one or more of the following conditions: no approval signature; no testing seal of SGS; no cross-page seal; altered; a copy without the red testing seal of SGS.
2. Above information and sample(s) was/were submitted and certified by the client, SGS quoted the information with no responsibility as to the accuracy, adequacy and/or completeness.
3. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested. This document cannot be used for publicity, without prior written approval of the SGS.
4. The test report cannot be reproduced in any way, except in full content, without prior approval in writing by the laboratory.
5. Should you have any queries or objection to the test report, please contact us within 15 days after receiving the report.

Address:

SGS Center, No.143, Zhuzhou Road, Laoshan District, Qingdao, China.

Tel: 0532-68999187

Zip: 266101

Fax: 0532-80991952

E-mail: Emily.Zhang@sgs.com

SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.

Page 6 of 6

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.



SGS-CSTC Standards Technical Services (Qingdao) Co., Ltd.

SGS Center, No.143, Zhuzhou Road, Laoshan District, Qingdao, Shandong, China 266101

t (86-532) 68999888

www.sgsgroup.com.cn

sgs.china@sgs.com

QD

7442596

Member of the SGS Group (SGS SA)

TEST REPORT

Report No. : CH:TX:9420026599-1

DATE : 19/12/2018



SHANDONG INTOCO MEDICAL PRODUCTS CO., LTD
9888, QIWANG ROAD, NAOSHAN INDUSTRY PARK,
QINGZHOU, SHANGDONG,
CHINA
A/C F615001 SGS CSTC STANDARDS TECHNICAL SERVICES CO. LTD
CONTACT PERSON : --

THE FOLLOWING SAMPLE(S) WAS/WERE SUBMITTED AND IDENTIFIED BY/ON BEHALF OF THE CUSTOMER AS :

SAMPLE DESCRIPTION GLOVES
DISPOSABLE NITRILE GLOVE
COLOUR BLUE
PRODUCT CODE 69702457560
PHOTO APPENDIX.



SAMPLE RECD ON 22/05/2018 **TESTING PERIOD :** 22/05/2018 - 29/05/2018

Summary of Test Results/Conclusion

| Test Method / Standard | Clause/Test Name | Status / Performance Level |
|------------------------|------------------------------------------------------------------------------|----------------------------|
| EN 16523-1:2015 | Permeation by Liquid chemical under conditions of continuous contact. | |
| | Formaldehyde 37% | Level - 3 |

Per pro SGS India Private Ltd.



K. PACHAIYAPPAN
ASST. MANAGER

Email your Test Report Related Enquiries at Feedback.SLT@sgs.com

Test report revised to add product code & reporting details as per customer request.

This Report cancels and supersedes the Report No 9420026599 Dated 30/05/2018 issued by SGS India.

TEST REPORT

Report No. : CH:TX:9420026599-1

DATE : 19/12/2018



RESULTS

EN 16523-1:2015 Determination of material resistance to permeation by chemicals – Part-1: Permeation by Liquid chemical under conditions of Continuous contact.


| Chemical CAS NO | Loop system/collection medium | Analytical technique used | Mean thickness (mm) | NBT at NPR $1.0 \mu\text{g cm}^{-2} \text{min}^{-1}$ (minutes) | Performance level accordance to EN ISO 374-1: 2016 Table 1 | Observation |
|--------------------------------|-------------------------------|--------------------------------------|----------------------|----------------------------------------------------------------|------------------------------------------------------------|-------------------|
| Formaldehyde 37% 50-00-0 | Closed loop/ Grade 3 water | Periodic measurement with HPLC | 0.11 0.10 0.10 | 65 70 68 | Level - 3 | Moderate Swelling |

EN ISO 374-1:2016 – Protective gloves against dangerous chemicals and micro-organisms.
Part 1: Terminology and performance requirements for chemical risks.
Table 1: Permeation performance levels.

| Permeation performance level | Measured breakthrough time (minutes) |
|------------------------------|--------------------------------------|
| 1 | >10 |
| 2 | >30 |
| 3 | >60 |
| 4 | >120 |
| 5 | >240 |
| 6 | >480 |

Performance levels are based on the lowest individual results achieved per chemical

Formaldehyde 37% Permeation Graph

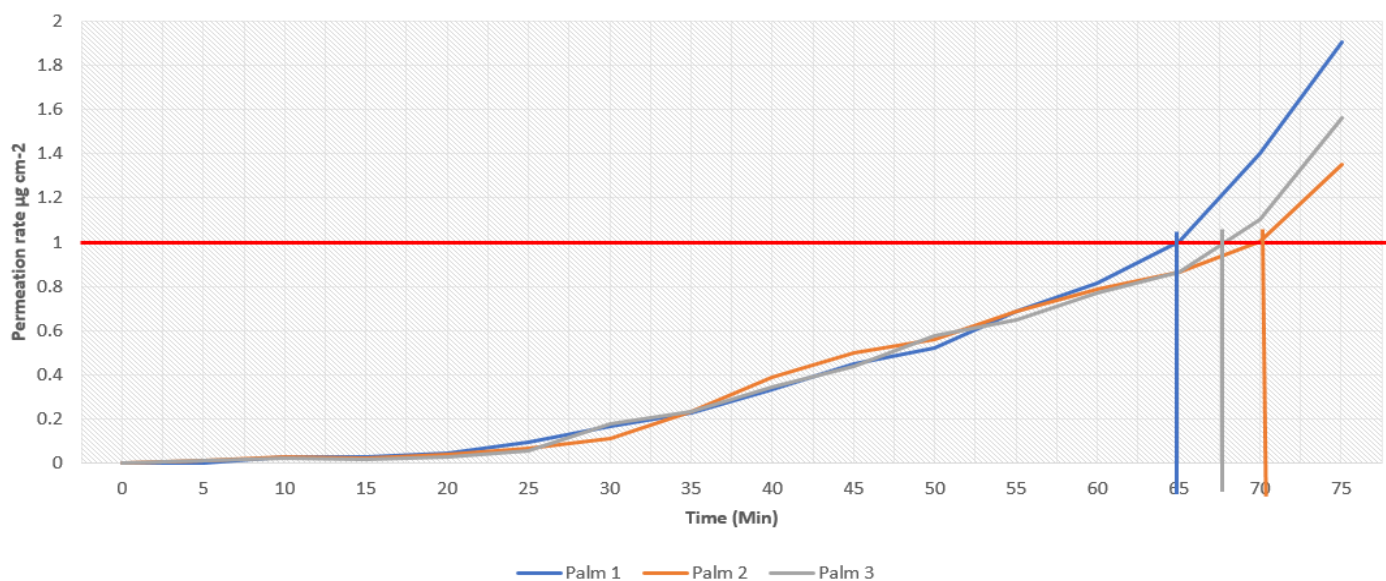

***** End of Report*****

TEST REPORT

Report No. : CH:TX:9420026316-1

DATE : 19/12/2018



SHANDONG INTCO MEDICAL PRODUCTS CO., LTD
9888, QIWANG ROAD, NAOSHAN INDUSTRY PARK,
QINGZHOU, SHANGDONG,
CHINA
A/C F615001 SGS CSTC STANDARDS TECHNICAL SERVICES CO. LTD
CONTACT PERSON : --

THE FOLLOWING SAMPLE(S) WAS/WERE SUBMITTED AND IDENTIFIED BY/ON BEHALF OF THE CUSTOMER AS :

SAMPLE DESCRIPTION GLOVES
DISPOSABLE NITRILE GLOVE
COLOUR BLUE
PRODUCT CODE 69702457560
PHOTO APPENDIX.



SAMPLE RECD ON 22/05/2018 **TESTING PERIOD :** 22/05/2018 - 29/05/2018

Summary of Test Results/Conclusion

| Test Method / Standard | Clause/Test Name | Status / Performance Level |
|------------------------|------------------------------------------------------------------------------|----------------------------|
| EN 16523-1:2015 | Permeation by Liquid chemical under conditions of continuous contact. | |
| | Hydrogen peroxide 30% | Level - 2 |

Per pro SGS India Private Ltd.

K. Pachaiyappan

K. PACHAIYAPPAN
ASST. MANAGER

Email your Test Report Related Enquiries at Feedback.SLT@sgs.com

Test report revised to add product code & reporting details as per customer request.

This Report cancels and supersedes the Report No 9420026316 Dated 29/05/2018 issued by SGS India.

TEST REPORT

Report No. : CH:TX:9420026316-1

DATE : 19/12/2018



RESULTS

EN 16523-1:2015 Determination of material resistance to permeation by chemicals – Part-1: Permeation by Liquid chemical under conditions of Continuous contact.


| Chemical CAS NO | Loop system/collection medium | Analytical technique used | Mean thickness (mm) | NBT at NPR 1.0 µg cm ⁻² min ⁻¹ (minutes) | Performance level accordance to EN ISO 374-1: 2016 Table 1 | Observation |
|---------------------------------|-------------------------------|---------------------------------------------|----------------------|----------------------------------------------------------------|------------------------------------------------------------|-------------------|
| Hydrogen Peroxide 30% 7722-84-1 | Closed loop/ Grade 3 water | Continuous measurement with Redox Electrode | 0.10 0.09 0.09 | 45 39 41 | Level - 2 | Moderate Swelling |

EN ISO 374-1:2016 – Protective gloves against dangerous chemicals and micro-organisms.
Part 1: Terminology and performance requirements for chemical risks.
Table 1: Permeation performance levels.

| Permeation performance level | Measured breakthrough time (minutes) |
|------------------------------|--------------------------------------|
| 1 | >10 |
| 2 | >30 |
| 3 | >60 |
| 4 | >120 |
| 5 | >240 |
| 6 | >480 |

Performance levels are based on the lowest individual results achieved per chemical.

Hydrogen Peroxide 30% Permeation Graph

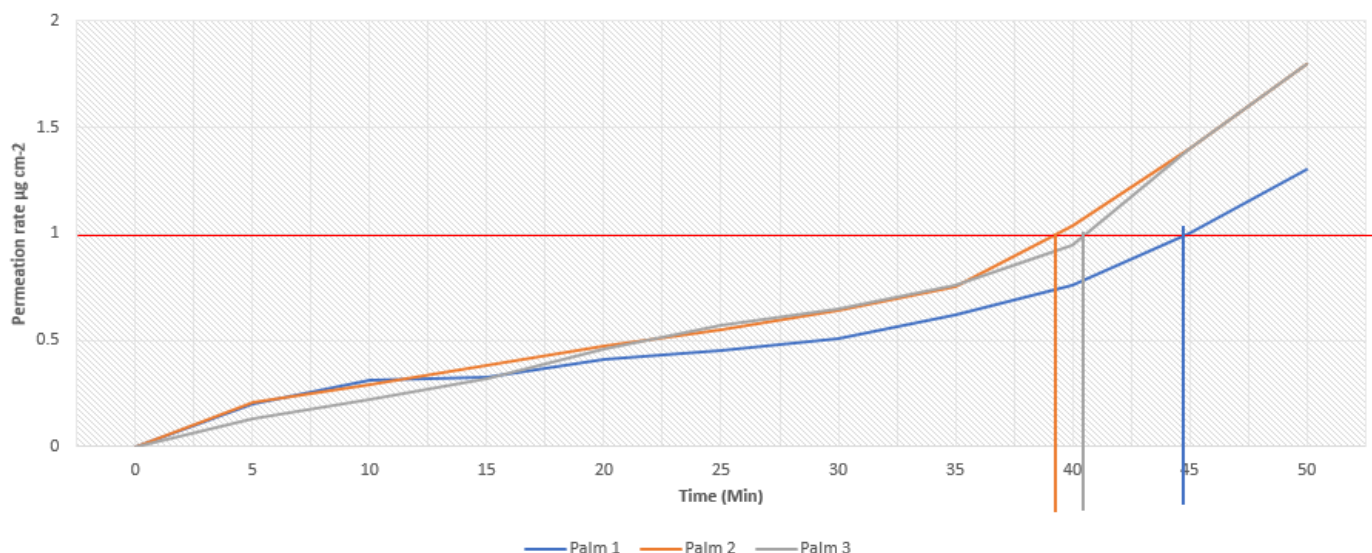

***** End of Report*****



SATRA Technology Centre Ltd
Wyndham Way, Telford Way, Kettering,
Northamptonshire, NN16 8SD United Kingdom
Tel: +44 (0) 1536 410000
Fax +44 (0) 1536 410626
email: info@satra.com
www.satra.com



Customer details: SATRA Technology Europe Ltd
Bracetown Business Park
Clonee
County Meath
Dublin 15
Eire

SATRA reference: CHM0295494/2009/JH

Your reference: STE0293607

Date of report: 4th March 2020

Samples received: 24th February 2020

Date(s) work carried out: 25th to 27th February 2020

TECHNICAL REPORT

SATRA Technology Europe Ltd: Certificate Number: 2777/11804-01/E00-00
Customer: Shandong Intco Medical Products Co Ltd
Qiwang Road, Naoshan Industrial Park
Qingzhou
Shandong
China
262506

Subject: Regulation 2016/425 Module C2 testing of gloves described as 697024575 Disposable Nitrile Non-Sterile Glove in accordance with EN 16523-1:2015+A1:2018 resistance to permeation by chemicals against 40% Sodium hydroxide .

Conditions of Issue:

This report may be forwarded to other parties provided that it is not changed in any way. It must not be published, for example by including it in advertisements, without the prior, written permission of SATRA.

Results given in this report refer only to the samples submitted for analysis and tested by SATRA. Comments are for guidance only.

Tests marked \neq fall outside the UKAS Accreditation Schedule for SATRA. All interpretations of results of such tests and the comments based upon them are outside the scope of UKAS accreditation and are based on current SATRA knowledge.

A satisfactory test report in no way implies that the product tested is approved by SATRA and no warranty is given as to the performance of the product tested. SATRA shall not be liable for any subsequent loss or damage incurred by the client as a result of information supplied in the report.

The uncertainty of the results (UoM) in this report is based on a standard uncertainty multiplied by a coverage factor $k=2$, which provides a coverage probability of approximately 95%.

Report signed by: Jade Hurley
Position: Technologist
Department: Chemical & Analytical Technology

(Page 1 of 6)

WORK REQUESTED:

Samples of gloves described as 697024575 Disposable Nitrile Non-Sterile Glove were obtained by SATRA Technology Europe Ltd from Shandong Intco Medical Products Co Ltd via SATRA Technology Services (Dongguan) Ltd on the 21st February 2020, in glove size Medium. The gloves were received by SATRA Technology UK on the 24th February 2020 for testing in accordance with EN 16523-1:2015+A1:2018 and with the performance requirements of EN ISO 374-1:2016+A1:2018 to demonstrate ongoing production compliance with Module C2 of Regulation (EU) 2016/425. These gloves are certified by certificate number 2777/11804-01/E00-00

SAMPLES SUBMITTED:



Samples described as 697024575
Disposable Nitrile Non-Sterile Glove

CONCLUSION:

When assessed in accordance with the requirements of EN ISO 374-1:2016+A1:2018 the samples of gloves described as 697024575 Disposable Nitrile Non-Sterile Glove achieved the following performance levels:

| Chemical | Performance level |
|---------------------------------------|-------------------|
| 40% Sodium hydroxide (CAS: 1310-73-2) | 6 |

Full results are reported in the following tables.



TESTING REQUIRED:

- EN 16523-1:2015+A1:2018 - Determination of material resistance to permeation by chemicals - Part 1: Permeation by liquid chemical under conditions of continuous contact


RESULTS AND REQUIREMENTS:

EN ISO 374-1:2016+A1:2018 - Protective gloves against dangerous chemicals and micro-organisms - Part 1: Terminology and performance requirements for chemical risks. Table 1: Permeation performance levels.

| Permeation performance level | Measured breakthrough time (minutes) |
|------------------------------|--------------------------------------|
| 1 | >10 |
| 2 | >30 |
| 3 | >60 |
| 4 | >120 |
| 5 | >240 |
| 6 | >480 |

Performance levels are based on the lowest individual result achieved per chemical.

| Test/Property | Sample reference: | 697024575 Disposable Nitrile Non-Sterile Glove | | Performance |
|--------------------------------------------------------------------------------------------------------------------------------------|--------------------------|--------------------------------------------------------------------------------------|---------------------------------|----------------|
| <p>EN 16523-1:2015 +A1:2018 in accordance with SATRA SOP CAT-009</p> <p>Using PTFE permeation cells with standardised dimensions</p> | Test information: | Chemical: 40% Sodium hydroxide | | Level 6 |
| | | Normalised permeation rate (NPR): 1 µg/cm ² /min | | |
| | | Detection technique: Conductimetry (continuous measurement) | | |
| | | Collection medium: Deionised water (closed loop) | | |
| | | Collection medium stirring rate: 45 – 65 ml/min (each cell constant to within ± 10%) | | |
| | | Test temperature: (23 ± 1) °C | | |
| | Specimen | Thickness (mm)^Δ | Breakthrough time (mins) | |
| | 1 | 0.07 | >480 | |
| | 2 | 0.06 | >480 | |
| | 3 | 0.06 | >480 | |
| | Test result: | >480 | | |
| | UoM: | <1 | | |
| Visual appearance of specimens after testing: | | Discoloured | | |

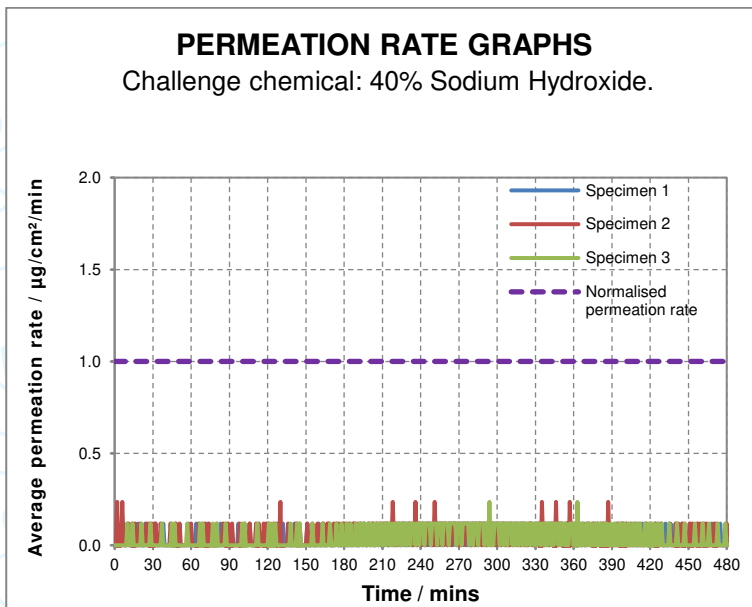

Δ EN 16523-1:2015+A1:2018 does not require the test specimen thicknesses to be reported, this information is indicative only.

TERMS AND CONDITIONS FOR THE SALE OF GOODS AND/OR THE PROVISION OF SERVICES

1. GENERAL

- 1.1 Work done, Services undertaken or the sale of Goods are subject to the terms and conditions detailed below and (subject to clause 5.2) all other conditions, warranties and representations, expressed or implied by statute relating thereto are hereby excluded.
- 1.2 SATRA Technology Centre Limited, its subsidiaries and associated companies (hereinafter referred to as "SATRA") may perform Services for or supply Goods to persons or entities (public, private or governmental) issuing instructions (hereinafter termed the "Client"). Each also known individually as a Party, or jointly as Parties.
- 1.3 These terms and conditions will apply to the Contract between SATRA and the Client to the exclusion of any other terms which the Client may seek to impose or which may be implied by trade, custom, practice or course of dealing
- 1.4 Unless otherwise agreed in writing no party other than the Client is entitled to provide instructions or information relating to the Goods or Services required or to the delivery of goods, results, reports or certificates.
- 1.5 All references in these terms and conditions to:
 - (a) the "Contract" is the contract between SATRA and the Client for the supply of Goods or Services which is made subject to these terms and conditions; and
 - (b) "Services" are the work or services to be supplied or performed under the Contract (including where relevant the supply of software, components and consumables); and
 - (c) "Goods" are the equipment, consumables or other physical items sold under the Contract (including documents, drawings or other information required in order to operate the equipment).
- 1.6 All drawings, descriptive matter, specifications and advertising material (including brochures and catalogues) are issued or published with the sole purpose of giving an indication of the goods or services being described and shall not form part of the Contract.
- 1.7 Where SATRA and the Client agree that the sale of Goods shall be governed by Incoterms 2010 (or any subsequent revision thereto) then the sale shall be governed by the relevant Incoterms mode of transport which is agreed by SATRA and the Client.

2. FEES AND PAYMENT

- 2.1 Where SATRA has agreed to perform the Services or supply the Goods on the basis of credit then payment terms are net 21 days from date of invoice, unless otherwise specified and may require part payment prior to delivery of the Services or Goods. In the event of the Client failing to make payment as agreed SATRA will be entitled to withhold delivery of the Goods or Services or cancel the Contract. SATRA reserves the right to charge interest on any overdue payments at a rate of 1.5% per month accruing on a daily basis from the date the invoice is due until the date payment is received.
- 2.2 Where the provision of Services or the sale of Goods is subject to a proforma invoice then SATRA shall not be obliged to start working on the provision of the Goods or Services until after payment in full has been made as cleared funds to SATRA.
- 2.3 SATRA reserves the right to charge for any and all expenses incurred as a result of performing the Services required by the Client. Although SATRA will try and provide an estimate of such expenses these may change as a result of circumstances out of SATRA's control.
- 2.4 Unless otherwise agreed in writing, the price for the Goods or Services shall be the price set in the order acknowledgement. SATRA shall not be bound by any price quoted which is not in writing. Prices for the sale of Goods include packing cases and materials but not carriage or installation which will be quoted separately and as agreed with the Client.
- 2.5 Quotations are valid from the date of issue for a period of 90 days unless otherwise specified or agreed in writing.
- 2.6 Should the Client become insolvent, bankrupt, subject to an administration order, enter into liquidation or receivership, or make arrangements with creditors SATRA reserves the right to cancel the Contract and terminate the supply of the Goods or Services. Where the Contract with SATRA is terminated all outstanding monies due from the Client to SATRA shall be immediately payable, and any materials supplied by SATRA to the Client returned. Termination of the Contract shall be without prejudice to any of SATRA's accrued rights.
- 2.7 All invoices issued by SATRA are payable in full. The Client is responsible for payment of withholding and any other taxes and all import duties. Payments made to SATRA shall not be reduced by such amounts.
- 2.8 The Client shall not be entitled to withhold or defer payment due to SATRA as a result of any dispute or counter claim that it may allege against SATRA.
- 2.9 SATRA reserves the right to bring action against the Client in order to collect unpaid fees, including court action. All fees associated with such actions shall be paid for by the Client including legal fees and related costs.
- 2.10 Where unforeseen costs arise as a result of provision of the Goods or carrying out the Services SATRA shall inform the Client immediately but reserves the right to charge additional costs to cover said costs and expenses.

3. INTELLECTUAL PROPERTY RIGHTS

- 3.1 All intellectual property rights belonging to a Party prior to entry into the Contract shall remain with that Party. Nothing in this Contract shall allow transfer of any intellectual property rights from one Party to the other.
- 3.2 In the event of certification services the use of certification marks by the Client may be subject to national and international laws and regulations. The responsibility for the use of these certification marks lies solely with the Client.
- 3.3 All intellectual property rights in reports, drawings, graphs, charts, photographs or any other material (in whatever medium) produced by SATRA pursuant to this Contract shall belong to SATRA. The Client shall have the right to use said material in accordance with the terms of this Contract.
- 3.4 The Client agrees and acknowledges that SATRA retains any and all proprietary rights in concepts, ideas and inventions that may arise during the preparation or provision of any report (including any deliverables provided by SATRA to the Client) and the provision of the Services to the Client.
- 3.5 All intellectual property rights in any software supplied to the Client shall belong to SATRA or SATRA's licensors. With respect to the sale of SATRA Timeline, SATRASUMM and SATRA Visionsitch, provided that the Client is a member of SATRA and has paid its annual Smartcare fee then the Client will be entitled to use the software for its own internal use and will be entitled to receive minor software upgrades and fixes. SATRA may however terminate the supply of software upgrades and fixes for older versions of software which it no longer considers viable to support. The Client's rights to use the software and receive software upgrades and fixes will terminate if the Client has not paid its annual Smartcare fee. Major upgrades are not included within the entitlement to upgrades but may be offered by SATRA from time to time for an additional fee.
- 3.6 SATRA shall observe all statutory provisions with regard to data protection including but not limited to the provisions of the Data Protection Act 2018 and the EU General Data Protection Regulation (GDPR) Regulation (EU) 2016/679. To the extent that SATRA processes or gets access to personal data in connection with the Services or otherwise in connection with this Contract, it shall take all reasonable technical and organisational measures to ensure the security of such data (and guard against unauthorised or unlawful processing, accidental loss, destruction or damage to such data).

4. SUSPENSION OR TERMINATION OF SERVICES

- 4.1 Cancellation by the Client of orders for Goods or Services will only be acceptable by prior agreement with SATRA and a charge will usually be made.
- 4.2 SATRA shall not be liable for any delay or failure in providing the Goods or Services due to circumstances beyond its reasonable control (including any failure by the Client to comply with its obligations). If any such circumstances arise which prevent SATRA from delivering the Goods or completing the Services, then SATRA will be entitled to cancel or reschedule the delivery of Goods or Services at its discretion. In the event of cancellation SATRA will be entitled to retain all fees paid by the Client for Goods or Services already supplied but will refund to the Client any fees paid by the Client for Goods or Services which have not yet been supplied. The Client will not be liable for any non-refundable expenses already incurred by SATRA in relation to Goods or Services not yet supplied unless the cancellation is due to the Client's failure to comply with its obligations under the Contract.

5. LIABILITY AND INDEMNIFICATION

- 5.1 Reports are issued on the basis of information, documents and/or samples submitted to SATRA by the Client, or on behalf of the Client and are provided solely for the benefit of the Client who is responsible for acting as it sees fit on the basis of such reports and findings. Subject to clause 5.2, neither SATRA nor any of its employees, agents or subcontractors shall be liable to the Client or any third party for any actions taken or not taken on the basis of such findings and reports, nor for any incorrect results arising as a result of unclear, erroneous, incomplete, misleading or false information provided to SATRA.
- 5.2 Nothing in these terms and conditions shall limit or exclude SATRA's liability for:
 - (a) death or personal injury caused by its negligence or the negligence of its employees or agents;
 - (b) fraud or fraudulent misrepresentation;
 - (c) breach of the terms implied by Section 12 of the Sale of Goods Act 1979;
 - (d) defective products under the Consumer Protection Act 1987; or
 - (e) any other liability which cannot be limited or excluded by applicable law.
- 5.3 Subject to clause 5.2 SATRA shall not be liable to the Client whether in contract, tort (including negligence), breach of statutory duty or otherwise arising under or in connection with the Contract for loss of profits, sales, contracts, anticipated savings, loss or damage to goodwill or any indirect or consequential loss.
- 5.4 Subject to clause 5.2 SATRA's total aggregate liability to the Client, whether in contract, tort (including negligence), breach of statutory duty or otherwise arising under or in connection with the Contract shall be limited to the total amount of fees for the Services or the price of the Goods (excluding any value added tax or other sales tax or expenses) payable by the Client to SATRA under the Contract or £100,000 whichever is the lower figure.

6. MISCELLANEOUS

- 6.1 If any one or more provisions of these conditions are found to be illegal or unenforceable in any respect, the validity, legality and enforceability of the remaining provisions shall not in any way be affected or impaired thereby.
 - 6.2 During the course of providing the Goods or Services and for a period of one year thereafter the Client shall not directly or indirectly entice, encourage or make any offer to SATRA's employees to leave their employment with SATRA.
 - 6.3 The use of SATRA's corporate name or registered marks for advertising purposes is not permitted without SATRA's prior written authorisation.
 - 6.4 All reports and documentation which are supplied to the Client under the Contract remain the property of SATRA until paid in full. Under no circumstances will a Client's purchase order override SATRA's retention of title in accordance with this clause.
 - 6.5 The Client acknowledges that in entering into this Contract it has not relied on any representation, warranty, collateral contract or other assurance (except those set out or referred to in these terms and conditions) made by or on behalf of SATRA or any other party before entering into the Contract. The Client waives all rights and remedies that, but for this clause, might otherwise be available to it in respect of any such representation, warranty, collateral contract or other assurance.
 - 6.6 All provisions of the Contract that limit or exclude the liability of SATRA are intended also to be for the benefit of SATRA's holding company (called SATRA, and being a company limited by guarantee and incorporated in England and Wales with company number 00153475), and shall accordingly be enforceable by such holding company as well as or instead of by SATRA, and on the basis that any limit on the liability of SATRA shall apply to it and to such holding company in the aggregate.
- ### 7. CONFIDENTIALITY
- 7.1 Unless specifically excluded in the terms of an individual contract between SATRA and the Client, the following shall apply to all deliverables including, reports, advice, drawings, photographs, specifications, data or other forms of media.
 - 7.2 Deliverables referred to in clause 7.1 shall not be disclosed to third parties or used in litigation without the consent of SATRA.
 - 7.3 Where SATRA has given consent to disclosure of any service deliverables referred to in clause 7.1, the Client shall draw the attention of the third party to these terms of business and the basis on which SATRA undertakes testing, reporting and advising. The Client shall indemnify SATRA for any failure to do so.
 - 7.4 The service deliverables referred to in clause 7.1 are submitted to the Client as confidential documents. Confidentiality shall continue to apply after completion of the business, but shall cease to apply to information or knowledge which has come into the public domain through no breach of this Contract by the Client.
 - 7.5 The Client shall not disassemble, remove parts or carry out any form of analysis on goods or materials sold by SATRA for the purposes of reverse engineering or obtaining information on the construction, content or composition of the item without the consent of SATRA.
- ### 8. AMENDMENT
- 8.1 No amendment to this Contract shall be effective unless it is in writing, expressly stated to amend this Contract and signed by an authorised signatory of both Parties.
- ### 9. DISPUTE RESOLUTION
- 9.1 If there should be a dispute between the parties to this Agreement they undertake to act with goodwill and to use all reasonable endeavours to resolve that dispute.
 - 9.2 Failure to resolve any dispute by discussions between the parties shall, in the first instance, be referred to a mediator for resolution. The parties shall attempt to agree upon the appointment of a mediator, upon receipt, by either of them, of a written notice to concur in such appointment. Should the parties fail to agree within 21 days, either party, upon giving written notice, may apply to the President or the Vice President, for the time being, of the Chartered Institute of Arbitrators, for the appointment of a mediator.
 - 9.3 Should the mediation fail, in whole or in part, either party may, upon giving written notice, and within twenty-eight days thereof, apply to the President or the Vice President, for the time being, of the Chartered Institute of Arbitrators, for the appointment of a single arbitrator, for final resolution. The arbitrator shall have no connection with the mediator or the mediation proceedings, unless both parties have consented in writing. The arbitration shall be governed by both the Arbitration Act 1996 and the Controlled Cost Rules of the

SATRA Technology Europe Ltd

SATRA Reference: CHM0295494/2009/JH

Date: 4th March 2020


Signed:



TERMS AND CONDITIONS FOR THE SALE OF GOODS AND/OR THE PROVISION OF SERVICES

- Chartered Institute of Arbitrators (2000 Edition), or any amendments thereof, which Rules are deemed to be incorporated by reference into this clause. The seat of the arbitration shall be England and Wales.
- 9.4 The laws of England shall govern the interpretation of this Contract. Subject to clauses 9.1, 9.2 and 9.3 any dispute arising out of or in connection with the Contract shall be subject to the exclusive jurisdiction of the courts of England. However, the Party obtaining a judgement in such courts shall be entitled to enforce it in any court it chooses.
- 10. PROVISION OF SERVICES**
- 10.1 SATRA shall provide Services using reasonable care and skill and in accordance with the Clients specific instructions and as confirmed by SATRA as part of the Contract review process.
- 10.2 Estimates for completion of the Services are made in good faith and date from receipt of a written order, payment of a proforma invoice if required, full information and samples to enable SATRA to proceed. While SATRA will make every effort to fulfil them, such estimates are subject to unforeseen events and if not achieved, cannot give rise to any claim. Time will not be of the essence in relation to the performance of the Services.
- 10.3 Results given in test reports or certificates refer only to samples submitted for analysis to SATRA. A satisfactory test report in no way implies that the product tested is approved by SATRA and no warranty is given as to the performance of the product tested.
- 10.4 SATRA may delegate all or part of the Services to a subcontractor and the Client authorises SATRA to disclose all information required to undertake the Services.
- 10.5 Where the Client requests SATRA to witness testing of other services being undertaken by a third party the Client agrees that SATRA's sole responsibility is to be present at the time of the work and to forward the results or confirm that the service has been undertaken. The Client agrees that unless otherwise agreed SATRA is not responsible for the condition or calibration of any equipment unless provided by SATRA.
- 10.6 Unless otherwise agreed in advance, test samples will be retained for 6 weeks from the date of the final report after which time they will be disposed of and SATRA shall cease to have any responsibility for such samples.
- Where the nature of the samples or the Services undertaken results in specialist disposal then SATRA reserves the right to pass the cost of such disposal onto the Client. Storage for longer periods may be possible only if agreed in advance and may incur a storage charge payable by the Client.
- Where practical and agreed in advance, samples may be returned at the Client's expense. However, samples are in most instances partially or fully destroyed as part of the work undertaken and SATRA cannot guarantee that samples will be returned in an "as new" condition.
- 10.7 Where SATRA receives documents reflecting engagements between the Client and third parties or documents belonging to third parties, such documents shall be considered as being for information only and shall not release the Client from any or all obligations to SATRA.
- 10.8 SATRA reserves the right to make changes to the Services, provided that such changes do not materially affect the nature or quality of the provision of these Services or where they are necessary in order to ensure that any applicable laws or safety requirements are complied with.
- 10.9 The Client acknowledges that SATRA by providing the Services, neither takes the place of the Client or any third party or releases them from any of their obligations.
- 11. CLIENT RESPONSIBILITIES RELATING TO THE PROVISION OF SERVICES**
- 11.1 The Client shall provide sufficient samples, information, instructions and documents as required to enable SATRA to carry out the Services in accordance with the methods, standards or other specifications as agreed.
- 11.2 Where applicable the Client shall allow access by members of SATRA staff to such premises where the Services are to be performed and provide any specialist equipment and personnel.
- 11.3 The Client shall inform SATRA in advance of any known hazards, dangers or other safety matters relating to samples submitted to SATRA or on site visits made by SATRA.
- 11.4 Where the Client fails to comply with any of its responsibilities SATRA reserves the right to suspend any Services until such time as the Client has complied and may require the Client to reimburse SATRA the amount of any additional costs arising from the suspension.
- 12. DELIVERY AND NON-DELIVERY OF GOODS**
- 12.1 Delivery dates for the supply of the Goods are approximate only and not guaranteed. Time of delivery is not of the essence of the Contract and SATRA shall not be liable for any delay in delivery of Goods.
- 12.2 Should expedited delivery be requested and agreed, SATRA shall be entitled to make additional charges to cover overtime or any other additional costs.
- 12.3 Delivery of the Goods shall take place at such location as SATRA and the Client agree. If the Client agrees to collect the Goods from SATRA's premises, then delivery will take place at those premises in which case the consignment of Goods as recorded by SATRA upon dispatch shall be evidence of the Goods received by the Client unless the Client can provide conclusive evidence to the contrary.
- 12.4 SATRA shall not be liable for the non-delivery of Goods (even if caused by SATRA) unless the Client provides written notice of non-delivery in accordance with clause 13.2. Liability for non-delivery of Goods shall in any event be limited to replacing the Goods within a reasonable time frame or the issue of a credit note to the value of the Goods not delivered.
- 12.5 Should delivery of the Goods be suspended or delayed by the Client for any reason SATRA reserves the right to charge for storage and for all expenses incurred, including loss of or wastage of resources that cannot otherwise be used. If the delay extends beyond 30 days SATRA shall be entitled to immediate payment for any Goods that are ready for delivery, and any other additional costs.
- 12.6 If for any reason the Client fails to accept delivery of any of the Goods when they are ready for delivery, or SATRA is unable to deliver the Goods on time because the Client has not provided appropriate instructions, documents, licenses or authorisations then risk in the Goods shall pass to the Client, the Goods and/or Services shall be deemed to have been delivered; and SATRA may store the Goods until delivery, whereupon the Client shall be liable for all related costs and expenses (including, without limitation, storage and insurance).
- 13. RISK/TITLE OF GOODS**
- 13.1 Subject to clause 12.6 the risk in the Goods will transfer to the Client on delivery of the Goods unless SATRA and the Client have agreed that the sale of the Goods will be governed by Incoterms 2010 (or any subsequent revision thereto) in which case risk will transfer to the Client in accordance with the Incoterms mode of transport which is agreed by SATRA and the Client.
- 13.2 The Company shall not accept responsibility for loss or damage in transit unless:
- a) In the case of sales where delivery of Goods is made in the United Kingdom SATRA is notified by the Client within 10 days of the invoice date of non-arrival of Goods and within 3 days of the invoice date of receipt of Goods damaged in transit; or
- b) In all other cases the Client notifies SATRA on the non-arrival or damage in transit within a reasonable period of time as determined by SATRA.
- 13.3 Title to the Goods shall not pass to the Client until the earlier of when: -
- a) SATRA receives payment in full (in cash or cleared funds) for the Goods and any other Goods that SATRA has supplied to the Client in which case title to the Goods shall pass at the time of payment of all such sums; and
- b) the Client resells the Goods in accordance with clause 13.5 in which case title shall pass to the Client immediately before the time at which the resale by the Client occurs.
- 13.4 Until ownership of Goods has passed to the Client, the Client shall:
- a) hold the Goods as SATRA's bailee;
- b) store the Goods (at no cost to SATRA) separately from all other goods belonging to the Client or any third party in such a way that they remain readily identifiable as SATRA's property (including where the Goods have been sold to a 3rd party);
- c) not destroy, deface or obscure any identifying mark or packaging on or relating to the Goods; and
- d) maintain the Goods in satisfactory condition and keep them insured on SATRA's behalf for their full price against all risks to the reasonable satisfaction of SATRA. The Client shall obtain an endorsement of SATRA's interest in the goods on its insurance policy. On request the Client shall allow SATRA to inspect such Goods and shall produce the policy of insurance.
- 13.5 The Client may resell the Goods before ownership has passed to it solely on condition that sale shall be effected in the ordinary course of the Client's business at full market value.
- 13.6 If before title to the Goods passes to the Client, the Client becomes subject to any of the events referred to in clause 2.6 then without limiting any other right or remedy SATRA may have:
- a) the Client's right to resell the Goods or use them in the ordinary course of its business ceases immediately; and
- b) SATRA may at any time require the Client to deliver up all Goods in its possession that have not been resold or irrevocably incorporated into another product; and
- c) if the Client fails to do so promptly SATRA may exercise its rights under clause 13.7.
- 13.7 The Client grants SATRA, its agents and employees an irrevocable licence at any time to enter any premises where the Goods are or may be stored in order to inspect them, or, where the Client's right to possession has terminated, to recover them.
- 13.8 On termination of the Contract, howsoever caused, SATRA's (but not the Client's) rights contained in this clause 13 shall remain in effect.
- 14. PATENTS**
- 14.1 SATRA gives no indemnity against any claim of infringement of Letters Patent, Registered Design, Trade Mark or Copyright by the use of or sale of any article or material supplied to the Client. If its use is impossible without infringement of Letters Patent, Registered Design, Trade Mark or Copyright published at the date of the contract, SATRA will refund to the Client the purchase price of the said article or material provided that it is returned to SATRA free of charge. The Client warrants that any design or instruction furnished or given by the Client shall not be such as will cause SATRA to infringe any Letters Patent, Registered Design, Trade Mark or Copyright in the execution of the Client's order.
- 15. WARRANTY OF GOODS**
- 15.1 SATRA warrants that on delivery and for a period of 12 months from the date of delivery or within the shelf life of the Goods (whichever is the shorter period) the Goods shall be free from defects in design, material and workmanship.
- 16. DEFECTIVE GOODS**
- 16.1 Subject to clauses 16.6 and 16.7 if:
- a) the Client gives notice in writing to SATRA in accordance with clause 16.3 and during the period referred to in clause 15.1 that the Goods do not comply with the warranty in that clause; and
- b) SATRA is given a reasonable opportunity of examining such Goods; and
- c) the Client (if asked to do so by SATRA) returns such Goods to SATRA's place of business then SATRA will, at its option, repair or replace the defective Goods or refund the price of the defective Goods in full. SATRA reserves the right to repair the Goods at the Client's premises.
- 16.2 The Client must inspect all Goods upon delivery. Failure to do so may result in further charges being applied in the event of a return.
- 16.3 If Goods are found to be faulty, defective or damaged the Client must inform SATRA in writing as soon as reasonably possible and in any event within 10 working days of the fault, damage or defect being discovered.
- 16.4 Without prejudice to clause 16.1 if no notice of rejection has been received by SATRA within 3 months of delivery, the Client shall be deemed to have accepted the Goods.
- 16.5 SATRA will pay the reasonable costs of carriage, packaging and insurance for any defective Goods which are returned by the Client provided that SATRA is liable under clause 16.1 to repair or replace the defective Goods. If SATRA determines that the Goods are not defective or if SATRA is not liable to repair or replace the Goods due to the circumstances under clauses 16.6 or 16.7 then the Client will be responsible for the payment of such costs.
- 16.6 SATRA shall not be under any liability to repair or at its option replace or pay for the repair or replacement of any Goods which are found to be defective if:
- a) the defect is caused or substantially caused by wear and tear, overloading, misuse, neglect, modification or attempted modification carried out by any organisation other than by SATRA or their approved agents, or use with ancillary equipment not approved in writing by SATRA, or default in proper maintenance or cleaning; or
- b) the Client authorises or carries out any repair or replacement of any Goods without first affording SATRA a reasonable opportunity to replace or repair them; or
- c) the Client has breached any of the terms of the Contract under which the Goods were supplied; or
- d) the Goods have been manufactured to a design or specification or in compliance with other information provided by the Client and the defect has arisen as a result of that design, specification or information;
- 16.7 Where Goods or parts of Goods are not manufactured by SATRA then SATRA shall be liable for defects only to the extent that SATRA obtains redress from the manufacturer or supplier thereof provided that:
- a) SATRA shall not be obliged to take any step to attempt to obtain such redress except at the request and expense of the Client and upon provision by the Client of a full indemnity as to costs for which SATRA may thereby become liable;
- b) nothing in this condition 16.7 shall have effect as to impose upon SATRA any additional liability or obligations other than those referred to in condition 16.1.
- 16.8 Except as provided in clause 16.1 SATRA shall have no liability to the Client arising from any failure of the Goods to comply with the warranty in clause 15.1.

Terms and conditions – September 2019

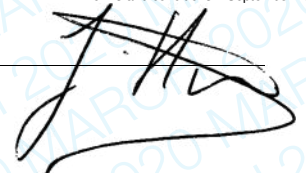

Signed:

SATRA Technology Europe Ltd
 SATRA Reference: CHM0295494/2009/JH
 Date: 4th March 2020

(Page 6 of 6)



TEST REPORT

C.C: SHANDONG INTCO MEDICAL PRODUCTS CO LTD
ADDRESS: NO. 9888 QIWANG ROAD, NAOSHAN INDUSTRY PARK, QINGZHOU, SHANDONG, CHINA

LAB NO.: (9021)060-0218
DATE IN: MAR. 01, 2020
DATE MODIFIED: /
DATE OUT: MAR. 09, 2020
NO. OF WORKING DAYS: 7
PAGE 1 OF 13

OVERALL RATING

| | |
|-----------------------|----------------------|
| SATISFACTORY | _____ X _____ |
| UNSATISFACTORY | _____ |
| DATA | _____ |

| | | | |
|--------------------------------|----------------------------------------|------------------------------|---|
| Vendor: | SHANDONG INTCO MEDICAL PRODUCTS CO LTD | Agent: | / |
| Raw Material Supplier: | / | Factory/Manufacturer: | / |
| P.O. No.: | / | Style No.: | / |
| Sample Description: | DISPOSABLE NITRILE GLOVES (NBR) | SKU#: | / |
| Color: | / | Country of Origin: | / |
| Buyer Name: | / | Submitted Size: | / |
| Submitted Amount: | / | End Use: | / |
| Country of Distribution | / | Others: | / |

| | |
|-----------------------------|-----------|
| Product Category: | / |
| Test Requested: | SEE BELOW |
| Previous Report No.: | / |

| TEST PROPERTY | PASS | FAIL | DATA | COMMENTS |
|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------|------|------|----------|
| Candidate List of Substances of Very High Concern for authorization published by European Chemicals Agency (ECHA) Regarding Regulation (EC) No. 1907/2006 concerning REACH | X | | | |

Remark:

The client specifies the test method and requirement.

BVCPS (SHANGHAI)-QINGDAO BRANCH CONTACT INFORMATION FOR THIS REPORT

Enquiry and invoicing:

Wendy Huang 86-533-7868187 wendy.huang@bureauveritas.com
Sunnee Li 86-533-7868185 sunnee.li@bureauveritas.com

Bureau Veritas
Consumer Products Services (Shanghai)-Qingdao Branch



Anderson Zhang
Qingdao Hardline Reporting Manager

Note:

1. The limit of 0.1% (w/w) applies to an article. The results were calculated according to Guidance on requirements for substances in articles Version 4.0 – June 2017, reference to the judgement of the European Court of Justice of 10 September 2015 in case C-106/142. However, the results may not be applicable if the intended use of the sample is a substance or mixture. According to REACH, definition of an article, substance and mixture are:
 - i. Article - An object during production is given a special shape, surface or design which determines its function to a greater degree than does its chemical composition
 - ii Substance - A chemical element and its compound in the natural state or obtained by any manufacturing process
 - iii Mixture (Previously known as "Preparation") - A mixture or solution composed of two or more substances
2. In accordance of Article 7 of Regulation (EC) No. 1907/2006 (REACH regulation) – Registration and notification of substances in articles, any producer or importer of articles shall notify ECHA, if a substance meets in criteria in Article 57 and is identified in accordance with Article 59(1), if both (1) the substance is present in those articles in quantities totalling over 1 tonne per producer or importer per year & (2) the substance is present in those articles above a concentration of 0.1% weight by weight (w/w) are met. The information to be notified shall include (a) identity and contact details of the producer or importer, (b) the registration numbers, (c) the identity of the substance and (d) the classification of the substance, (e) a brief description of the use of the substance and (f) the tonnage range of the substance.
3. In accordance of Article 33 of Regulation (EC) No. 1907/2006 (REACH regulation) – Duty to communicate information on substances in articles, any supplier of an article containing a substance meeting the criteria in Article 57 and identified in accordance with Article 59(1) in concentration above 0.1% weight by weight (w/w) shall provide the recipient of the article with sufficient information, available to the supplier, to allow safe use of the article including, as a minimum, the name of that substance. On request by a consumer the relevant information shall be provided by any supplier of an article free of charge, within 45 days of receipt of the request.
4. If SVHC was detected exceeding 0,1% (w/w) in test group, client is suggested to perform the further separate testing to identify the exact concentration of test items.

Bureau Veritas Consumer Products Services, Inc. (Shanghai), Qingdao Branch
No.3 building, GNDC Tech Base, No.192 Zhuzhou Road, Laoshan District, Qingdao, China, 266101
Tel: 86-532-58827999 Fax: 86-532-88706839
Email: bvcpsinfor.qd@cn.bureauveritas.com
Website: cps.bureauveritas.com

This report is governed by, and incorporates by reference, CPS Conditions of Service as posted at the date of issuance of this report at <http://www.bureauveritas.com/home/about-us/our-business/cps/about-us/terms-conditions> and is intended for your exclusive use. Any copying or replication of this report to or for any other person or entity, or use of our name or trademark, is permitted only with our prior written permission. This report sets forth our findings solely with respect to the test samples identified herein. The results set forth in this report are not indicative or representative of the quality or characteristics of the lot from which a test sample was taken or any similar or identical product unless specifically and expressly noted. Our report includes all of the tests requested by you and the results thereof based upon the information that you provided to us. Measurement uncertainty is only provided upon request for accredited tests. You have 60 days from date of issuance of this report to notify us of any material error or omission caused by our negligence or if you require measurement uncertainty; provided, however, that such notice shall be in writing and shall specifically address the issue you wish to raise. A failure to raise such issue within the prescribed time shall constitute your unqualified acceptance of the completeness of this report, the tests conducted and the correctness of the report contents.

TEST RESULT

Candidate List of Substances of Very High Concern for authorization published by European Chemicals Agency (ECHA) Regarding Regulation (EC) No. 1907/2006 concerning REACH

Method: Analysis is based on GC, LC, IC, ICP and UV, with various detection techniques.

| | |
|---------------------------------|------------------------------|
| Maximum Allowable Limit: | 0.1% (Each of listed) |
|---------------------------------|------------------------------|

| | |
|--------------------|--------------|
| Test Item1: | Blue Plastic |
|--------------------|--------------|

| Result | | Conclusion |
|---------------------|-----------|------------|
| Detected Analyte(s) | Conc. (%) | |
| ND | ND | PASS |

Remark:

ND = Not Detected
 mg/kg = milligram per kilogram
 Detection Limit (%): See Appendix.
 The detected SVHC and its value will be shown in above table, the else SVHC not shown in the table will be regarded as ND. When all SVHC for test are not detected, it will be shown ND.

Conc. = Concentration
 % = percentage
 1 mg/kg = 0.0001%

APPENDIX

Candidate List of Substances of Very High Concern for authorization published by European Chemicals Agency (ECHA) Regarding Regulation (EC) No. 1907/2006 concerning REACH

| No. | Substance name | CAS No. | EC No. | Detection Limit, % | Basis for identification as a SVHC |
|-----|-------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------|-------------------------|--------------------|-------------------------------------------------------|
| 1 | Triethyl arsenate* | 15606-95-8 | 427-700-2 | 0.01 | Carcinogenic |
| 2 | Anthracene | 120-12-7 | 204-371-1 | 0.005 | PBT |
| 3 | 4,4'-Diaminodiphenyl methane (MDA) | 101-77-9 | 202-974-4 | 0.005 | Carcinogenic |
| 4 | Dibutyl phthalate (DBP) | 84-74-2 | 201-557-4 | 0.005 | Toxic for reproduction |
| 5 | Cobalt dichloride* | 7646-79-9 | 231-589-4 | 0.01 | Carcinogenic |
| 6 | Diarsenic pentaoxide* | 1303-28-2 | 215-116-9 | 0.01 | Carcinogenic |
| 7 | Diarsenic trioxide* | 1327-53-3 | 215-481-4 | 0.01 | Carcinogenic |
| 8 | Sodium dichromate* | 7789-12-0 ⁽¹⁾ , 10588-01-9 ⁽²⁾ | 234-190-3 | 0.01 | Carcinogenic; Mutagenic; Toxic for reproduction |
| 9 | 5-tert-butyl-2,4,6-trinitro-m-xylene (musk xylene) | 81-15-2 | 201-329-4 | 0.005 | vPvB |
| 10 | Bis (2-ethylhexyl) phthalate (DEHP) | 117-81-7 | 204-211-0 | 0.005 | Toxic for reproduction |
| 11 | Hexabromo cyclododecane (HBCDD) and all major diastereoisomers identified: α - HBCDD β - HBCDD γ - HBCDD | 3194-55-6 ⁽³⁾ , 25637-99-4 ⁽⁴⁾ 134237-50-6 134237-51-7 134237-52-8 | 247-148-4, 221-695-9 | 0.005 | PBT |
| 12 | Alkanes, C10-13, chloro (Short Chain Chlorinated Paraffins) (SCCP) | 85535-84-8 | 287-476-5 | 0.01 | PBT, vPvB |

| | | | | | |
|----|-------------------------------------------------------------------|-------------------------------------------------|--------------------------|-------|-------------------------------------------------------|
| 13 | Bis(tributyltin)oxide (TBTO)** | 56-35-9 | 200-268-0 | 0.005 | PBT |
| 14 | Lead hydrogen arsenate* | 7784-40-9 | 232-064-2 | 0.01 | Carcinogenic; Toxic for reproduction |
| 15 | Benzyl butyl phthalate (BBP) | 85-68-7 | 201-622-7 | 0.005 | Toxic for reproduction |
| 16 | 2,4-Dinitrotoluene | 121-14-2 | 204-450-0 | 0.005 | Carcinogenic |
| 17 | Anthracene oil | 90640-80-5 | 292-602-7 | 0.01 | Carcinogenic, PBT, vPvB |
| 18 | Anthracene oil, anthracene paste, distn. Lights | 91995-17-4 | 295-278-5 | 0.01 | Carcinogenic; Mutagenic, PBT, vPvB |
| 19 | Anthracene oil, anthracene paste, anthracene fraction | 91995-15-2 | 295-275-9 | 0.01 | Carcinogenic; Mutagenic, PBT, vPvB |
| 20 | Anthracene oil, anthracene-low | 90640-82-7 | 292-604-8 | 0.01 | Carcinogenic; Mutagenic, PBT, vPvB |
| 21 | Anthracene oil, anthracene paste | 90640-81-6 | 292-603-2 | 0.01 | Carcinogenic; Mutagenic, PBT, vPvB |
| 22 | Diisobutyl phthalate | 84-69-5 | 201-553-2 | 0.005 | Toxic for reproduction |
| 23 | Aluminosilicate, Refractory Ceramic Fibres* ^a | Index no. 650-017-00-8 | | 0.01 | Carcinogenic |
| 24 | Zirconia Aluminosilicate, Refractory Ceramic Fibres* ^b | Index no. 650-017-00-8 | | 0.01 | Carcinogenic |
| 25 | Lead chromate* | 7758-97-6 | 231-846-0 | 0.01 | Carcinogenic; Toxic for reproduction |
| 26 | Lead chromate molybdate sulfate red (C.I. Pigment Red 104)* | 12656-85-8 | 235-759-9 | 0.01 | Carcinogenic; Toxic for reproduction |
| 27 | Lead sulfochromate yellow (C.I. Pigment Yellow 34)* | 1344-37-2 | 215-693-7 | 0.01 | Carcinogenic; Toxic for reproduction |
| 28 | Tris(2-chloroethyl) phosphate (TCEP) | 115-96-8 | 204-118-5 | 0.005 | Toxic for reproduction |
| 29 | Coal tar pitch, high temperature | 65996-93-2 | 266-028-2 | 0.01 | Carcinogenic, PBT, vPvB |
| 30 | Acrylamide | 79-06-1 | 201-173-7 | 0.005 | Carcinogenic; Mutagenic |
| 31 | Trichloroethylene | 79-01-6 | 201-167-4 | 0.005 | Carcinogenic |
| 32 | Boric acid* | 10043-35-3, 11113-50-1 | 233-139-2 / 234-343-4 | 0.01 | Toxic for reproduction |
| 33 | Disodium tetraborate, anhydrous* | 1330-43-3(5), 12179-04-3(6), 1303-96-4(7) | 215-540-4 | 0.01 | Toxic for reproduction |
| 34 | Tetraboron disodium heptaoxide, hydrate* | 12267-73-1 | 235-541-3 | 0.01 | Toxic for reproduction |
| 35 | Sodium chromate* | 7775-11-3 | 231-889-5 | 0.01 | Carcinogenic; Mutagenic; Toxic for reproduction |
| 36 | Potassium chromate* | 7789-00-6 | 232-140-5 | 0.01 | Carcinogenic; Mutagenic |
| 37 | Ammonium dichromate* | 7789-09-5 | 232-143-1 | 0.01 | Carcinogenic; Mutagenic; Toxic for reproduction |
| 38 | Potassium dichromate* | 7778-50-9 | 231-906-6 | 0.01 | Carcinogenic; Mutagenic; Toxic for reproduction |
| 39 | Cobalt(II) sulphate* | 10124-43-3 | 233-334-2 | 0.01 | Carcinogenic; Toxic for reproduction |
| 40 | Cobalt(II) dinitrate* | 10141-05-6 | 233-402-1 | 0.01 | Carcinogenic; Toxic for reproduction |
| 41 | Cobalt(II) carbonate* | 513-79-1 | 208-169-4 | 0.01 | Carcinogenic; Toxic for reproduction |
| 42 | Cobalt(II) diacetate* | 71-48-7 | 200-755-8 | 0.01 | Carcinogenic; |

| | | | | | |
|----|-------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------|-----------------------------|-------|-----------------------------------------|
| | | | | | Toxic for reproduction |
| 43 | 2-Methoxyethanol | 109-86-4 | 203-713-7 | 0.005 | Toxic for reproduction |
| 44 | 2-Ethoxyethanol | 110-80-5 | 203-804-1 | 0.005 | Toxic for reproduction |
| 45 | Chromium trioxide* | 1333-82-0 | 215-607-8 | 0.01 | Carcinogenic; Mutagenic |
| 46 | Acid generated from chromium trioxide and their oligomers: Chromic acid* Dichromic acid* Oligomers of chromic acid and dichromic acid* | 7738-94-5 13530-68-2 - | 231-801-5 236-881-5 - | 0.01 | Carcinogenic |
| 47 | 2-Ethoxyethyl acetate | 111-15-9 | 203-839-2 | 0.005 | Toxic for reproduction |
| 48 | Strontium Chromate* | 7789-06-2 | 232-142-6 | 0.01 | Carcinogenic |
| 49 | 1,2-benzenedicarboxylic acid, di-C7-11 branched alkyl ester and linear alkyl ester | 68515-42-4 | 271-084-6 | 0.005 | Toxic for reproduction |
| 50 | Hydrazine | 302-01-2 7803-57-8 | 206-114-9 | 0.005 | Carcinogenic |
| 51 | 1-Methyl-2-pyrrolidone | 872-50-4 | 212-828-1 | 0.005 | Toxic for reproduction |
| 52 | 1,2,3-trichloropropane | 96-18-4 | 202-486-1 | 0.005 | Toxic for reproduction |
| 53 | 1,2-benzenedicarboxylic acid, di-C6-8-branched alkyl ester, C7-rich (DIHP) | 71888-89-6 | 276-158-1 | 0.005 | Toxic for reproduction |
| 54 | Dichromium tris(chromate)* | 24613-89-6 | 246-356-2 | 0.01 | Carcinogenic |
| 55 | Potassium hydroxyoctaoxodizincatedi-chromate* | 11103-86-9 | 234-329-8 | 0.01 | Carcinogenic |
| 56 | Pentazinc chromate octahydroxide* | 49663-84-5 | 256-418-0 | 0.01 | Carcinogenic |
| 57 | Formaldehyde, oligomeric reaction products with aniline (technical MDA) | 25214-70-4 | 500-036-1 | 0.005 | Carcinogenic |
| 58 | Bis(2-methoxyethyl) phthalate | 117-82-8 | 204-212-6 | 0.005 | Toxic for reproduction |
| 59 | 2-Methoxyaniline; o-Anisidine | 90-04-0 | 201-963-1 | 0.005 | Carcinogenic |
| 60 | 4-(1,1,3,3-tetramethylbutyl)phenol, (4-tert-Octylphenol) | 140-66-9 | 205-426-2 | 0.005 | Equivalent level of concern |
| 61 | 1,2-Dichloroethane | 107-06-2 | 203-458-1 | 0.005 | Carcinogenic |
| 62 | Bis(2-methoxyethyl) ether | 111-96-6 | 203-924-4 | 0.005 | Toxic for reproduction |
| 63 | Arsenic acid* | 7778-39-4 | 231-901-9 | 0.01 | Carcinogenic |
| 64 | Calcium arsenate* | 7778-44-1 | 231-904-5 | 0.01 | Carcinogenic |
| 65 | Trilead diarsenate* | 3687-31-8 | 222-979-5 | 0.01 | Carcinogenic; Toxic for reproduction |
| 66 | N,N-dimethylacetamide (DMAC) | 127-19-5 | 204-826-4 | 0.005 | Toxic for reproduction |
| 67 | 2,2'-dichloro-4,4'-methylenedianiline (MOCA) | 101-14-4 | 202-918-9 | 0.005 | Carcinogenic |
| 68 | Phenolphthalein | 77-09-8 | 201-004-7 | 0.005 | Carcinogenic |
| 69 | Lead azide, Lead diazide* | 13424-46-9 | 236-542-1 | 0.01 | Toxic for reproduction |
| 70 | Lead styphnate* | 15245-44-0 | 239-290-0 | 0.01 | Toxic for reproduction |
| 71 | Lead dipicrate* | 6477-64-1 | 229-335-2 | 0.01 | Toxic for reproduction |
| 72 | 1,2-bis(2-methoxyethoxy)ethane (TEGDME; triglyme) | 112-49-2 | 203-977-3 | 0.005 | Toxic for reproduction |
| 73 | 1,2-dimethoxyethane; ethylene glycol dimethyl ether (EGDME) | 110-71-4 | 203-794-9 | 0.005 | Toxic for reproduction |
| 74 | Diboron trioxide* | 1303-86-2 | 215-125-8 | 0.01 | Toxic for reproduction |
| 75 | Formamide | 75-12-7 | 200-842-0 | 0.01 | Toxic for reproduction |
| 76 | Lead(II) bis(methanesulfonate)* | 17570-76-2 | 401-750-5 | 0.01 | Toxic for reproduction |

| | | | | | |
|----|-----------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------|-----------------------------------------------------|-------|---------------------------------------------------------------------------------|
| 77 | TGIC (1,3,5-tris(oxiranylmethyl)-1,3,5-triazine-2,4,6(1H,3H,5H)-trione) § | 2451-62-9 | 219-514-3 | 0.005 | Mutagenic |
| 78 | β-TGIC (1,3,5-tris[(2S and 2R)-2,3-epoxypropyl]-1,3,5-triazine-2,4,6-(1H,3H,5H)-trione) § | 59653-74-6 | 423-400-0 | 0.005 | Mutagenic |
| 79 | 4,4'-bis(dimethylamino)benzophenone (Michler's ketone) | 90-94-8 | 202-027-5 | 0.005 | Carcinogenic |
| 80 | N,N,N',N'-tetramethyl-4,4'-methylenedianiline (Michler's base) | 101-61-1 | 202-959-2 | 0.005 | Carcinogenic |
| 81 | [4-[4,4'-bis(dimethylamino)benzhydrylidene]cyclohexa-2,5-dien-1-ylidene]dimethylammonium chloride (C.I. Basic Violet 3) | 548-62-9 | 208-953-6 | 0.005 | Carcinogenic |
| 82 | [4-[[4-anilino-1-naphthyl][4-(dimethylamino)phenyl]methylene]cyclohexa-2,5-dien-1-ylidene]dimethylammonium chloride (C.I. Basic Blue 26) | 2580-56-5 | 219-943-6 | 0.005 | Carcinogenic |
| 83 | α,α-Bis[4-(dimethylamino)phenyl]-4 (phenylamino)naphthalene-1-methanol (C.I. Solvent Blue 4) | 6786-83-0 | 229-851-8 | 0.01 | Carcinogenic |
| 84 | 4,4'-bis(dimethylamino)-4''-(methylamino)trityl alcohol | 561-41-1 | 209-218-2 | 0.005 | Carcinogenic |
| 85 | Bis(pentabromophenyl) ether (DecaBDE) | 1163-19-5 | 214-604-9 | 0.005 | Persistent, bioaccumulative and toxic; very persistent and very bioaccumulative |
| 86 | N,N-dimethylformamide; dimethyl formamide | 68-12-2 | 200-679-5 | 0.005 | Toxic for reproduction |
| 87 | Methoxy acetic acid | 625-45-6 | 210-894-6 | 0.005 | Toxic for reproduction ; equivalent level of concern |
| 88 | Dibutyltin dichloride (DBT)* | 683-18-1 | 211-670-0 | 0.01 | Toxic for reproduction |
| 89 | 1,2-Diethoxyethane | 629-14-1 | 211-076-1 | 0.005 | Toxic for reproduction |
| 90 | Hexahydro-2-benzofuran-1,3-dione (HHPA), cis-cyclohexane-1,2-dicarboxylic anhydride, trans-cyclohexane-1,2-dicarboxylic anhydride | 85-42-7, 13149-00-3, 14166-21-3 | 201-604-9, 236-086-3, 238-009-9 | 0.01 | Equivalent level of concern having probable serious effects to human health |
| 91 | Hexahydromethylphthalic anhydride, Hexahydro-4-methylphthalic anhydride, Hexahydro-1-methylphthalic anhydride, Hexahydro-3-methylphthalic anhydride | 25550-51-0, 19438-60-9, 48122-14-1, 57110-29-9 | 247-094-1, 243-072-0, 256-356-4, 260-566-1 | 0.01 | Equivalent level of concern having probable serious effects to human health |
| 92 | 4-Nonylphenol, branched and linear - substances with a linear and/or branched alkyl chain with a carbon number of 9 covalently bound in | - | - | 0.005 | Equivalent level of concern having probable serious effects to human health |

| | | | | | |
|-----|--------------------------------------------------------------------------------------------------------------------------------------------|-------------|-----------|-------|------------------------------------------|
| | position 4 to phenol, covering also UVCB- and well-defined substances which include any of the individual isomers or a combination thereof | | | | |
| 93 | Heptacosafuorotetradecanoic acid | 376-06-7 | 206-803-4 | 0.005 | Very persistent and very bioaccumulative |
| 94 | 1,2-Benzenedicarboxylic acid, dipentylester, branched and linear+ | 84777-06-0 | 284-032-2 | 0.005 | Toxic for reproduction |
| 95 | Henicosafuoroundecanoic acid | 2058-94-8 | 218-165-4 | 0.005 | Very persistent and very bioaccumulative |
| 96 | N-pentyl-isopentylphthalate (iPnPP)+ | 776297-69-9 | - | 0.005 | Toxic for reproduction |
| 97 | Pentacosafuorotridecanoic acid | 72629-94-8 | 276-745-2 | 0.005 | Very persistent and very bioaccumulative |
| 98 | 4-(1,1,3,3-tetramethylbutyl)phenol, ethoxylated - covering well-defined substances and UVCB substances, polymers and homologues | - | - | 0.005 | Equivalent level of concern |
| 99 | Tricosafuorododecanoic acid | 307-55-1 | 206-203-2 | 0.005 | Very persistent and very bioaccumulative |
| 100 | Lead bis(tetrafluoroborate)* | 13814-96-5 | 237-486-0 | 0.01 | Toxic for reproduction |
| 101 | Lead tetroxide (orange lead)* | 1314-41-6 | 215-235-6 | 0.01 | Toxic for reproduction |
| 102 | Diethyl sulphate | 64-67-5 | 200-589-6 | 0.005 | Carcinogenic; Mutagenic |
| 103 | Dinoseb | 88-85-7 | 201-861-7 | 0.005 | Toxic for reproduction |
| 104 | Lead Titanium Zirconium Oxide* | 12626-81-2 | 235-727-4 | 0.01 | Toxic for reproduction |
| 105 | Acetic acid, lead salt, basic* | 51404-69-4 | 257-175-3 | 0.01 | Toxic for reproduction |
| 106 | Furan | 110-00-9 | 203-727-3 | 0.01 | Carcinogenic |
| 107 | N-methylacetamide | 79-16-3 | 201-182-6 | 0.005 | Toxic for reproduction |
| 108 | o-Toluidine; 2-Aminotoluene | 95-53-4 | 202-429-0 | 0.005 | Carcinogenic |
| 109 | 3-ethyl-2-methyl-2-(3-methylbutyl)-1,3-oxazolidine | 143860-04-2 | 421-150-7 | 0.01 | Toxic for reproduction |
| 110 | 4,4'-oxydianiline and its salts | 101-80-4 | 202-977-0 | 0.005 | Carcinogenic; Mutagenic |
| 111 | [Phthalato(2-)]dioxotrilead (Dibasic lead phthalate)* | 69011-06-9 | 273-688-5 | 0.01 | Toxic for reproduction |
| 112 | Lead titanium trioxide* | 12060-00-3 | 235-038-9 | 0.01 | Toxic for reproduction |
| 113 | Lead oxide sulphate* | 12036-76-9 | 234-853-7 | 0.01 | Toxic for reproduction |
| 114 | Lead dinitrate* | 10099-74-8 | 233-245-9 | 0.01 | Toxic for reproduction |
| 115 | 4-Aminoazobenzene; 4-Phenylazoaniline | 60-09-3 | 200-453-6 | 0.005 | Carcinogenic |
| 116 | Lead cyanamidate* | 20837-86-9 | 244-073-9 | 0.01 | Toxic for reproduction |
| 117 | Tetralead trioxide sulphate* | 12202-17-4 | 235-380-9 | 0.01 | Toxic for reproduction |
| 118 | 4-methyl-m-phenylenediamine (2,4-toluene-diamine) | 95-80-7 | 202-453-1 | 0.005 | Carcinogenic |
| 119 | Pyrochlore, antimony lead yellow* | 8012-00-8 | 232-382-1 | 0.01 | Toxic for reproduction |
| 120 | Trilead bis(carbonate)dihydroxide (basic lead carbonate)* | 1319-46-6 | 215-290-6 | 0.01 | Toxic for reproduction |
| 121 | Dimethyl sulphate | 77-78-1 | 201-058-1 | 0.005 | Carcinogenic |
| 122 | Dioxobis(stearato)trilead* | 12578-12-0 | 235-702-8 | 0.01 | Toxic for reproduction |
| 123 | Silicic acid, barium salt, lead-doped* | 68784-75-8 | 272-271-5 | 0.01 | Toxic for reproduction |
| 124 | Biphenyl-4-ylamine | 92-67-1 | 202-177-1 | 0.005 | Carcinogenic |
| 125 | Lead oxide (lead monoxide)* | 1317-36-8 | 215-267-0 | 0.01 | Toxic for reproduction |
| 126 | Pentalead tetraoxide sulphate* | 12065-90-6 | 235-067-7 | 0.01 | Toxic for reproduction |
| 127 | Propylene oxide; 1,2-epoxypropane; methyloxirane | 75-56-9 | 200-879-2 | 0.01 | Carcinogenic; Mutagenic |
| 128 | Silicic acid, lead salt* | 11120-22-2 | 234-363-3 | 0.01 | Toxic for reproduction |

| | | | | | |
|-----|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------|-----------|-------|------------------------------------------------------------------------------------------------------------------------------|
| 129 | Trilead dioxide phosphonate* | 12141-20-7 | 235-252-2 | 0.01 | Toxic for reproduction |
| 130 | o-aminoazotoluene | 97-56-3 | 202-591-2 | 0.005 | Carcinogenic |
| 131 | 1-bromopropane | 106-94-5 | 203-445-0 | 0.01 | Toxic for reproduction |
| 132 | 6-methoxy-m-toluidine (p-cresidine) | 120-71-8 | 204-419-1 | 0.005 | Carcinogenic |
| 133 | 4,4'-methylenedi-o-toluidine | 838-88-0 | 212-658-8 | 0.005 | Carcinogenic |
| 134 | Tetraethyllead* | 78-00-2 | 201-075-4 | 0.01 | Toxic for reproduction |
| 135 | Sulfurous acid, lead salt, dibasic* | 62229-08-7 | 263-467-1 | 0.01 | Toxic for reproduction |
| 136 | Fatty acids, C16-18, lead salts* | 91031-62-8 | 292-966-7 | 0.01 | Toxic for reproduction |
| 137 | Diisopentylphthalate+ | 605-50-5 | 210-088-4 | 0.005 | Toxic for reproduction |
| 138 | Diazene-1,2-dicarboxamide (C,C'-azodi(formamide)) | 123-77-3 | 204-650-8 | 0.01 | Equivalent level of concern having probable serious effects to human health |
| 139 | Cadmium* | 7440-43-9 | 231-152-8 | 0.01 | Carcinogenic; Equivalent level of concern |
| 140 | Cadmium oxide* | 1306-19-0 | 215-146-2 | 0.01 | Carcinogenic; Equivalent level of concern |
| 141 | Dipentyl phthalate (DPP) + | 131-18-0 | 205-017-9 | 0.005 | Toxic for reproduction |
| 142 | 4-Nonylphenol, branched and linear, ethoxylated [substances with a linear and/or branched alkyl chain with a carbon number of 9 covalently bound in position 4 to phenol, ethoxylated covering UVCB- and well-defined substances, polymers and homologues, which include any of the individual isomers and/or combinations thereof] | - | - | 0.005 | Equivalent level of concern |
| 143 | Ammonium pentadecafluorooctanoate (APFO) ≠ | 3825-26-1 | 223-320-4 | 0.005 | Toxic for reproduction; PBT |
| 144 | Pentadecafluorooctanoic acid (PFOA) ≠ | 335-67-1 | 206-397-9 | 0.005 | Toxic for reproduction; PBT |
| 145 | Cadmium sulphide | 1306-23-6 | 215-147-8 | 0.01 | Carcinogenic; Equivalent level of concern |
| 146 | Dihexyl phthalate | 84-75-3 | 201-559-5 | 0.005 | Toxic for reproduction |
| 147 | Disodium 3,3'-[[1,1'-biphenyl]-4,4'-diylbis(azo)]bis(4-aminonaphthalene-1-sulphonate) (C.I. Direct Red 28) | 573-58-0 | 209-358-4 | 0.005 | Carcinogenic |
| 148 | Disodium 4-amino-3-[[4'-[(2,4-diaminophenyl)azo][1,1'-biphenyl]-4-yl]azo] -5-hydroxy-6-(phenylazo)naphthalene-2,7-disulphonate (C.I. Direct Black 38) | 1937-37-7 | 217-710-3 | 0.005 | Carcinogenic |
| 149 | Imidazolidine-2-thione (2-imidazoline-2-thiol) | 96-45-7 | 202-506-9 | 0.005 | Toxic for reproduction |
| 150 | Lead diacetate | 301-04-2 | 206-104-4 | 0.01 | Toxic for reproduction |
| 151 | Trixylyl phosphate | 25155-23-1 | 246-677-8 | 0.005 | Toxic for reproduction |
| 152 | Cadmium chloride* | 10108-64-2 | 233-296-7 | 0.01 | Carcinogenic; Mutagenic; Toxic for Reproduction; Equivalent level of concern having probable serious effects to human health |
| 153 | 1,2-Benzenedicarboxylic acid, dihexyl ester, branched and linear++ | 68515-50-4 | 271-093-5 | 0.005 | Toxic for reproduction |

| | | | | | |
|-----|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------|-------------------------|-------|------------------------------------------------------------------------------------------------------------------------------------|
| 154 | Sodium peroxometaborate* | 7632-04-4 | 231-556-4 | 0.01 | Toxic for reproduction |
| 155 | Sodium perborate; perboric acid, sodium salt* | - | 239-172-9; 234-390-0 | 0.01 | Toxic for reproduction |
| 156 | Cadmium fluoride * | 7790-79-6 | 232-222-0 | 0.01 | Carcinogenic; Mutagenic; Toxic for Reproduction; Equivalent level of concern having probable serious effects to human health |
| 157 | Cadmium sulphate * | 10124-36-4; 31119-53-6 | 233-331-6 | 0.01 | Carcinogenic; Mutagenic; Toxic for Reproduction; Equivalent level of concern having probable serious effects to human health |
| 158 | 2-benzotriazol-2-yl-4,6-di-tert-butylphenol (UV-320) | 3846-71-7 | 223-346-6 | 0.005 | PBT; vPvB |
| 159 | 2-(2H-benzotriazol-2-yl)-4,6-ditertpentylphenol (UV-328) | 25973-55-1 | 247-384-8 | 0.005 | PBT; vPvB |
| 160 | 2-ethylhexyl 10-ethyl-4,4-dioctyl-7-oxo-8-oxa-3,5-dithia-4-stannatetradecanoate (DOTE) +++ | 15571-58-1 | 239-622-4 | 0.01 | Toxic for Reproduction |
| 161 | Reaction mass of 2-ethylhexyl 10-ethyl-4,4-dioctyl-7-oxo-8-oxa-3,5-dithia-4-stannatetradecanoate and 2-ethylhexyl 10-ethyl-4-[[2-[(2-ethylhexyl)oxy]-2-oxoethyl]thio]-4-octyl-7-oxo-8-oxa-3,5-dithia-4-stannatetradecanoate (reaction mass of DOTE and MOTE) +++ | - | - | 0.01 | Toxic for Reproduction |
| 162 | 1,2-benzenedicarboxylic acid, di-C6-10-alkyl esters; 1,2-benzenedicarboxylic acid, mixed decyl and hexyl and octyl diesters with ≥ 0.3% of dihexyl phthalate (EC No. 201-559-5) | 68515-51-5; 68648-93-1 | 271-094-0; 272-013-1 | 0.01 | Toxic for reproduction |
| 163 | 5-sec-butyl-2-(2,4-dimethylcyclohex-3-en-1-yl)-5-methyl-1,3-dioxane [1], 5-sec-butyl-2-(4,6-dimethylcyclohex-3-en-1-yl)-5-methyl-1,3-dioxane [2] [covering any of the individual isomers of [1] and [2] or any combination thereof] | - | - | 0.01 | Very persistent and very bioaccumulative |
| 164 | 1,3-propanesultone | 1120-71-4 | 214-317-9 | 0.01 | Carcinogenic |
| 165 | 2,4-di-tert-butyl-6-(5-chlorobenzotriazol-2-yl)phenol (UV-327) | 3864-99-1 | 223-383-8 | 0.005 | vPvB |
| 166 | 2-(2H-benzotriazol-2-yl)-4-(tert-butyl)-6-(sec-butyl)phenol (UV-350) | 36437-37-3 | 253-037-1 | 0.005 | vPvB |
| 167 | Nitrobenzene | 98-95-3 | 202-716-0 | 0.01 | Toxic for reproduction |
| 168 | Perfluorononan-1-oic-acid and its sodium and ammonium salts | 375-95-1 21049-39-8 4149-60-4 | 206-801-3 | 0.01 | Toxic for reproduction; PBT |
| 169 | Benzo[def]chrysene (Benzo[a]pyrene) | 50-32-8 | 200-028-5 | 0.005 | Carcinogenic; Mutagenic; Toxic for Reproduction; PBT; vPvB |
| 170 | 4,4'-isopropylidenediphenol | 80-05-7 | 201-245-8 | 0.005 | Toxic for reproduction |

| | | | | | |
|-----|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------|-----------|-------|-----------------------------------------------------------------------------------|
| | (bisphenol A) | | | | Endocrine disrupting properties- environment & human health |
| 171 | Nonadecafluorodecanoic acid (PFDA) and its sodium and ammonium salts/ | - | - | 0.005 | Toxic for reproduction; PBT |
| 172 | 4-Heptylphenol, branched and linear [substances with a linear and/or branched alkyl chain with a carbon number of 7 covalently bound predominantly in position 4 to phenol, covering also UVCB- and well-defined substances which include any of the individual isomers or a combination thereof] | - | - | 0.005 | Equivalent level of concern having probable serious effects to the environment |
| 173 | p-(1,1-dimethylpropyl)phenol | 80-46-6 | 201-280-9 | 0.005 | Equivalent level of concern having probable serious effects to the environment |
| 174 | Perfluorohexane-1-sulphonic acid and its salts (PFHxS) | - | - | 0.005 | vPvB |
| 175 | Reaction products of 1,3,4-thiadiazolidine-2,5-dithione, formaldehyde and 4-heptylphenol, branched and linear (RP-HP) [with $\geq 0.1\%$ w/w 4-heptylphenol, branched and linear(4-HPbl)] | - | - | 0.01 | Endocrine disrupting properties- environment |
| 176 | Dodecachloropentacyclo[12.2.1.16, 9.02,13.05,10]octadeca-7,15-diene ("Dechlorane Plus" TM) [covering any of its individual anti- and syn-isomers or any combination thereof] | - | - | 0.01 | vPvB |
| 177 | Chrysene | 218-01-9 1719-03-5 | 205-923-4 | 0.005 | Carcinogenic; PBT; vPvB |
| 178 | Cadmium nitrate* | 10022-68-1 10325-94-7 | 233-710-6 | 0.01 | Carcinogenic; Mutagenic Specific target organ toxicity after repeated exposure |
| 179 | Cadmium hydroxide* | 21041-95-2 | 244-168-5 | 0.01 | Carcinogenic; Mutagenic Specific target organ toxicity after repeated exposure |
| 180 | Cadmium carbonate* | 513-78-0 | 208-168-9 | 0.01 | Carcinogenic; Mutagenic Specific target organ toxicity after repeated exposure |
| 181 | Benz[a]anthracene | 56-55-3 1718-53-2 | 200-280-6 | 0.005 | Carcinogenic; PBT; vPvB |
| 182 | Terphenyl, hydrogenated | 61788-32-7 | 262-967-7 | 0.005 | vPvB |
| 183 | Octamethylcyclotetrasiloxane(D4) | 556-67-2 | 209-136-7 | 0.005 | PBT; vPvB |
| 184 | Lead | 7439-92-1 | 231-100-4 | 0.01 | Toxic for reproduction |
| 185 | Ethylenediamine (EDA) | 107-15-3 | 203-468-6 | 0.005 | Respiratory sensitising |

| | | | | | properties |
|-----|--------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------|-----------|-------|----------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 186 | Dodecamethylcyclhexasiloxane (D6) | 540-97-6 | 208-762-8 | 0.005 | PBT; vPvB |
| 187 | Disodium octaborate* | 12008-41-2 | 234-541-0 | 0.005 | Toxic for reproduction |
| 188 | Dicyclohexyl phthalate (DCHP) | 84-61-7 | 201-545-9 | 0.005 | Toxic for reproduction; Endocrine disrupting properties |
| 189 | Decamethylcyclopentasiloxane (D5) | 541-02-6 | 208-764-9 | 0.005 | PBT; vPvB |
| 190 | Benzo[ghi]perylene | 191-24-2 | 205-883-8 | 0.005 | PBT; vPvB |
| 191 | Benzene-1,2,4- tricarboxylic acid 1,2 anhydride (TMA) | 552-30-7 | 209-008-0 | 0.005 | Respiratory sensitising properties |
| 192 | Pyrene | 129-00-0 1718-52-1 | 204-927-3 | 0.005 | PBT; vPvB |
| 193 | Phenanthrene | 85-01-8 | 201-581-5 | 0.005 | vPvB |
| 194 | Fluoranthene | 206-44-0 93951-69-0 | 205-912-4 | 0.005 | PBT; vPvB |
| 195 | Benzo[k]fluoranthene | 207-08-9 | 205-916-6 | 0.005 | Carcinogenic; PBT; vPvB |
| 196 | 2,2-bis(4'-hydroxyphenyl)-4-methylpentane | 6807-17-6 | 401-720-1 | 0.005 | Toxic for reproduction |
| 197 | 1,7,7-trimethyl-3-(phenylmethylene)-Bicyclo[2.2.1]heptan-2-one | 15087-24-8 | 239-139-9 | 0.005 | Endocrine disrupting properties |
| 198 | 2,3,3,3-tetrafluoro-2-(heptafluoropropoxy)propionic acid, its salts and its acyl halides (covering any of their individual isomers and combinations thereof) | - | - | 0.01 | Equivalent level of concern having probable serious effects to human health Equivalent level of concern having probable serious effects to the environment/ |
| 199 | 2-methoxyethyl acetate | 110-49-6 | 203-772-9 | 0.01 | Toxic for reproduction |
| 200 | Tris(4-nonylphenyl, branched and linear) phosphite (TNPP) with ≥ 0.1% w/w of 4-nonylphenol, branched and linear (4-NP) | - | - | 0.01 | Endocrine disrupting properties |
| 201 | 4-tert-butylphenol | 98-54-4 | 202-679-0 | 0.005 | Endocrine disrupting properties |
| 202 | 2-benzyl-2-dimethylamino-4'-morpholinobutyrophenone | 119313-12-1 | 404-360-3 | 0.005 | Toxic for reproduction |
| 203 | 2-methyl-1-(4-methylthiophenyl)-2-morpholinopropan-1-one | 71868-10-5 | 400-600-6 | 0.005 | Toxic for reproduction |
| 204 | Diisohexyl phthalate | 71850-09-4 | 276-090-2 | 0.005 | Toxic for reproduction |
| 205 | Perfluorobutane sulfonic acid (PFBS) and its salts | - | - | 0.005 | Equivalent level of concern having probable serious effects on the environment and human health/ |
| 206 | 1-vinylimidazole | 1072-63-5 | 214-012-0 | 0.005 | Toxic for reproduction |
| 207 | 2-methylimidazole | 693-98-1 | 211-765-7 | 0.005 | Toxic for reproduction |
| 208 | Dibutylbis(pentane-2,4-dionato-O,O')tin +++ | 22673-19-4 | 245-152-0 | 0.01 | Toxic for reproduction |
| 209 | Butyl 4-hydroxybenzoate | 94-26-8 | 202-318-7 | 0.005 | Equivalent level of concern having probable serious effects on the |

| | | | | | |
|-----|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------|-----------|------|------------------------------------------------|
| | | | | | human health - Endocrine disrupting properties |
| 210 | bis(2-(2-methoxyethoxy)ethyl) ether | 143-24-8 | 205-594-7 | 0.01 | Toxic for reproduction |
| 211 | Diocetyl tin dilaurate, stannane, dioctyl-, bis(coco acyloxy) derivs., and any other stannane, dioctyl-, bis(fatty acyloxy) derivs. wherein C12 is the predominant carbon number of the fatty acyloxy moiety | - | - | 0.01 | Toxic for reproduction |

- (1) CAS no. 7789-12-0 refers to sodium dichromate dihydrate
(2) CAS no. 10588-01-9 refers to anhydrous sodium dichromate
(3) CAS no. 3194-55-6 refers to a specific HBCDD - 1,2,5,6,9,10-hexabromocyclododecane
(4) CAS no. 25637-99-4 refers to unspecific HBCDD isomer composition
(5) CAS no. 1330-43-4 refers to disodium tetraborate, anhydrous
(6) CAS no. 12179-04-3 refers to sodium tetraborate, pentahydrate
(7) CAS no. 1303-96-4 refers to sodium tetraborate, decahydrate

Remark:

1. PBT = Persistent, bio accumulative and toxic as defined in Regulation (EC) No 1907/2006
2. vPvB = Very persistent and very bio accumulative as defined in Regulation (EC) No 1907/2006
3. ND = Not Detected
- *Result is based on the heavy metal or inorganic element concentration. Due to the limit of the analytical technology available, any further investigation is not feasible. The client is strongly advised to review the chemical formulation to ascertain.
- **Result is identified by tributyltin (TBT). Due to the limit of the analytical technology available, any further investigation is not feasible. The client is strongly advised to review the chemical formulation to ascertain.
- §TGIC (1,3,5-tris(oxiranylmethyl)-1,3,5-triazine-2,4,6(1H,3H,5H)-trione) and β-TGIC (1,3,5-tris[(2S and 2R)-2,3-epoxypropyl]-1,3,5-triazine-2,4,6-(1H,3H,5H)-trione) are reported as a mixture.
- ^aRefer to Aluminosilicate, Refractory Ceramic Fibres fulfil the three following conditions: a) oxides of aluminium and silicon are the main components present (in the fibres) within variable concentration ranges b) fibres have a length weighted geometric mean diameter less two standard geometric errors of 6 or less micrometres (µm) c) alkaline oxide and alkali earth oxide (Na₂O+K₂O+CaO+MgO+BaO) content less or equal to 18% by weight.
- ^bRefer to Zirconia Aluminosilicate, Refractory Ceramic Fibres fulfil the three following conditions: a) oxides of aluminium, silicon and zirconium are the main components present (in the fibres) within variable concentration ranges b) fibres have a length weighted geometric mean diameter less two standard geometric errors of 6 or less micrometres (µm). c) alkaline oxide and alkali earth oxide (Na₂O+K₂O+CaO+MgO+BaO) content less or equal to 18% by weight.
- ⁺[1,2-Benzenedicarboxylic acid, dipentylester, branched and linear] is a mixture of phthalates contains DPP, DIPP and N-pentyl-isopentylphtalate.
- [‡]PFOA and APFO are reported together. The result is based on PFOA concentration. Due to the limit of the analytical technology available, any further investigation is not feasible. The client is strongly advised to review the chemical formulation to ascertain.
- ⁺⁺[1,2-Benzenedicarboxylic acid, dihexyl ester, branched and linear] is a mixture of phthalates contains dihexyl phthalate.
- ⁺⁺⁺Result is based on the tin metal concentration, and further confirmation for checking DBT, DOTE & MOTE concentration.

Original Sample



END